

File ..ATA\2018\20180917\392\CPK2018-917-19826-1.D Tgt Mass (CHM):

Injection Date : 17 Sep 18 5:59 pm +0800 Seq. Line : 4

Sample Name : CPK2018-917-19826 Location : P2-C-09

Acq. Operator : LQ\_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.4 ul

Acq. Method : D:\Chem32\1\data\2018\20180917\392\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2018\20180917\392\1-POS-3MIN-1.M

SCatalog No: HY-12031 Batch#19826 A-RP-314

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

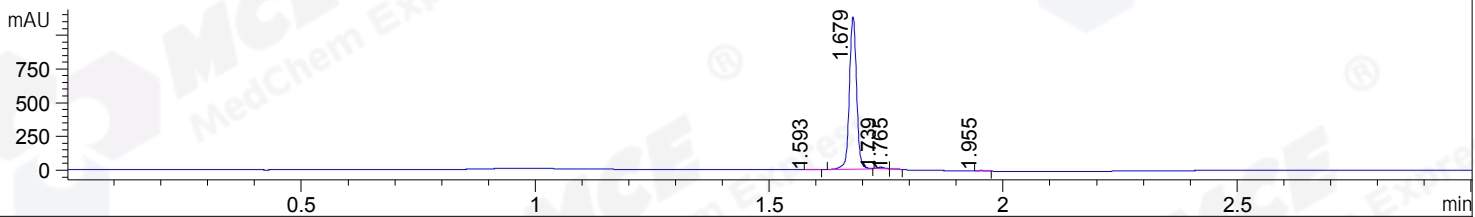


DAD1 C, Sig=254,4 Ref=off

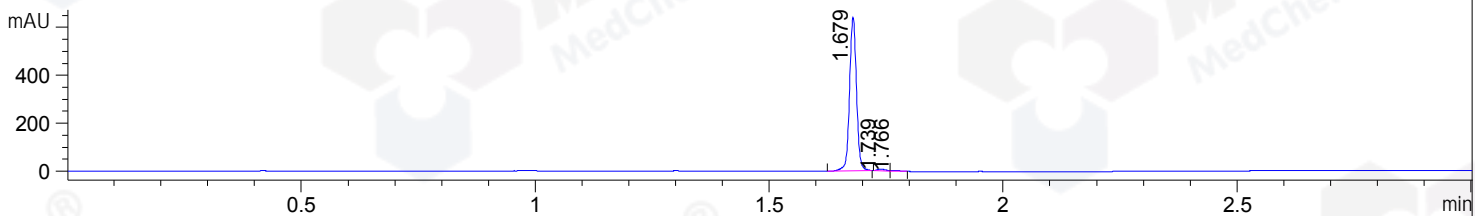

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

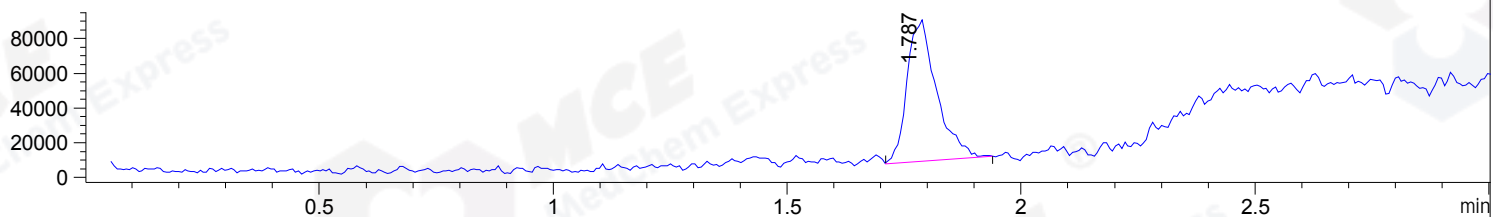

Ion 427.6, MSD1 427.6, Target Mass 426.6 +H Positive, EIC=427.3:428.3

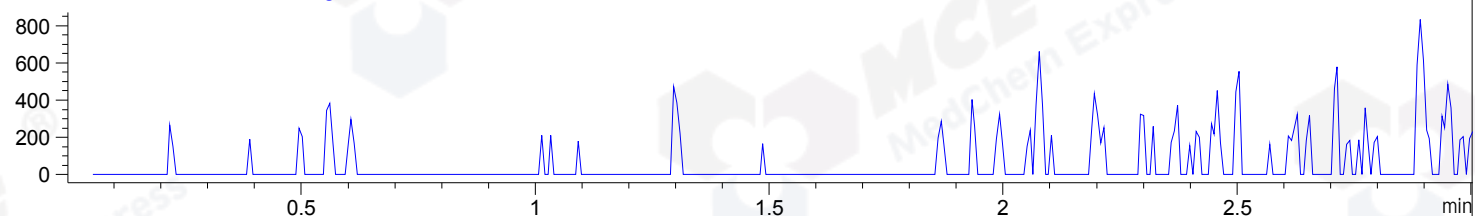

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.59	0.02	2.29	1.84	0.19	ND
1.68	0.02	1197.34	1128.92	98.06	ND
1.74	0.02	12.66	11.51	1.04	347
1.76	0.02	4.67	3.74	0.38	191
1.95	0.02	4.05	3.49	0.33	141

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.68	0.02	659.20	641.60	98.39	ND
1.74	0.02	7.76	6.55	1.16	347
1.77	0.02	3.03	2.26	0.45	191

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.79	0.06	357762.19	81899.38	100.00	347

Ret. Time: 1.79

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

