



File ..213 2019-12-13 17-00-55\CPK2019-D11-21369.D Tgt Mass (CHM):
 Injection Date : 13 Dec 19 8:19 pm +0800 Seq. Line : 37
 Sample Name : CPK2019-D11-21369 Location : P1-C-01
 Acq. Operator : SYSTEM Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\LCMS03\Data\20191213\20191213 2019-12-13 17-00-55\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20191213\20191213 2019-12-13 17-00-55\1-POS-3MIN.M
 Catalog No : HY-100036 Batch# 21369
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-446
 Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

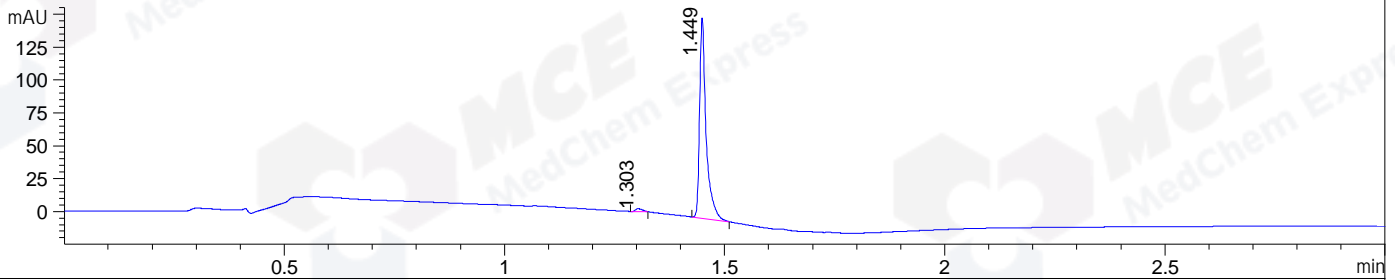

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

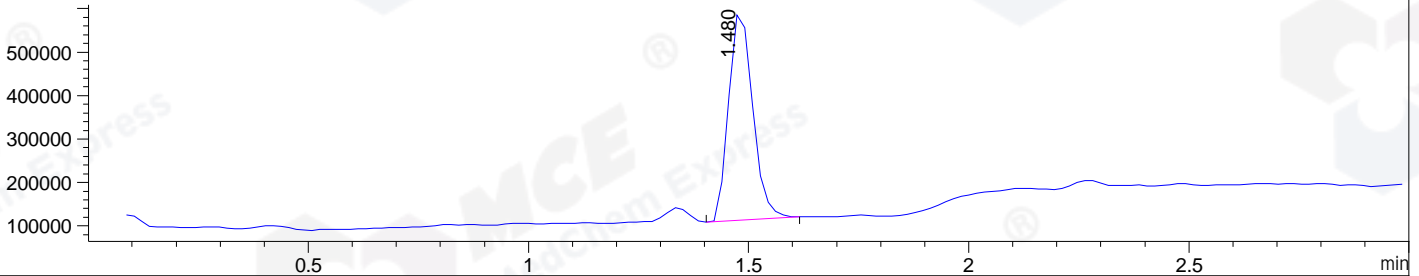

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

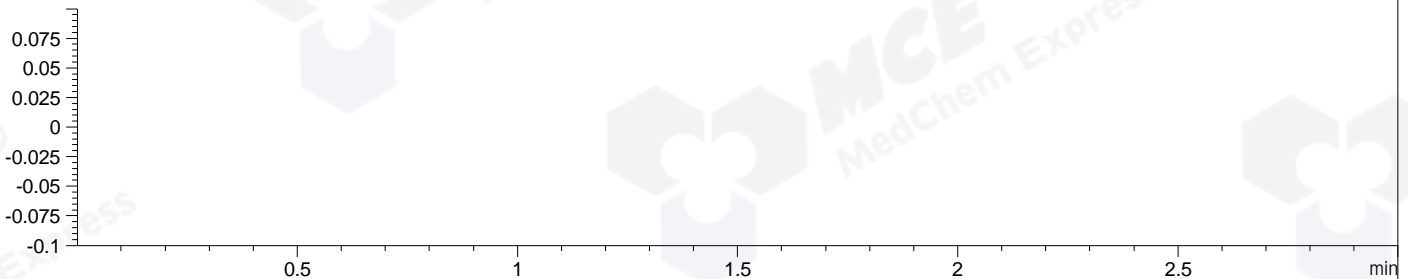

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.30	0.02	2.70	2.33	1.69	114
1.45	0.02	157.17	153.46	98.31	494

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.48	0.06	1813726.50	485701.50	100.00	494

Ret. Time: 1.48

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

