

File ..\DATA\2019\20190711\627\CPK2019-710-24029.D Tgt Mass (CHM):

Injection Date : 11 Jul 19 11:14 am +0800 Seq. Line : 32

Sample Name : CPK2019-710-24029 Location : P1-B-03

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190711\627\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190711\627\1-POS-3MIN.M

Catalog No : HY-10006 Batch#24029

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

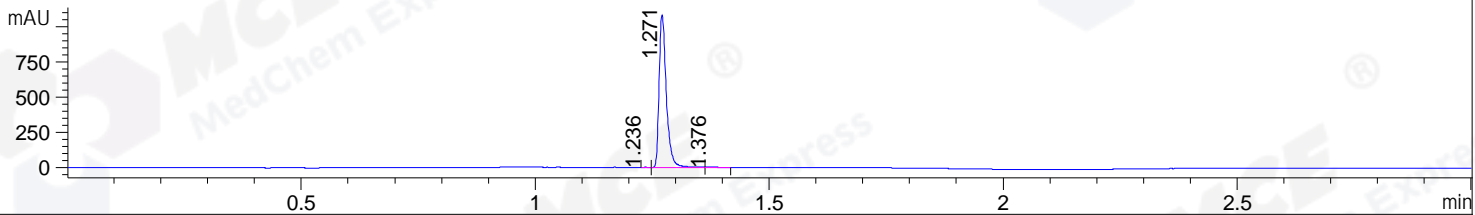


DAD1 C, Sig=254,4 Ref=off

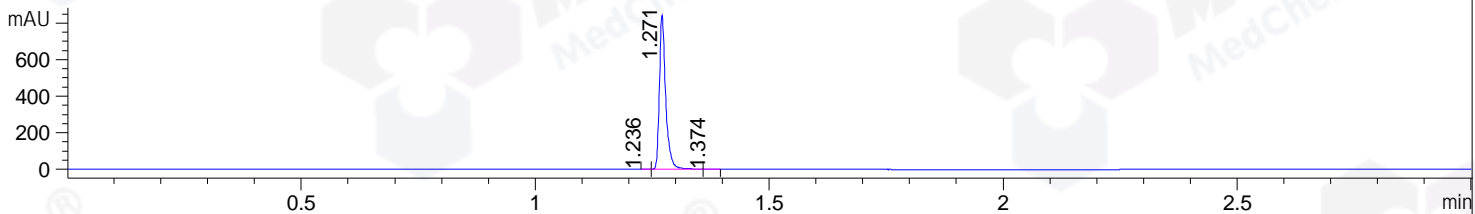

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

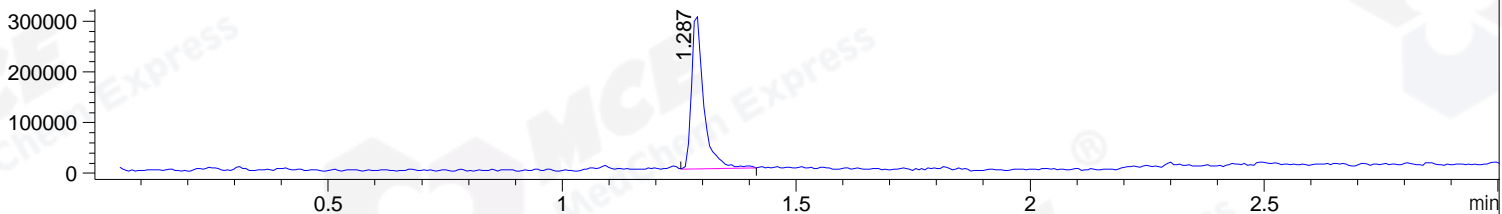

Ion 439.3112, MSD1 439.3112, Target Mass 438.3112 +H Positive, EIC=439.01:440.01

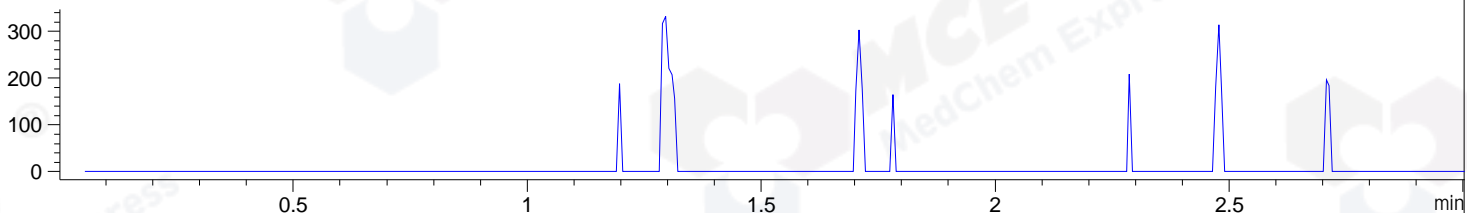

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.01	1.12	1.52	0.10	ND
1.27	0.02	1162.62	1084.20	99.64	402
1.38	0.02	3.11	2.15	0.27	402

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.01	0.75	0.97	0.09	ND
1.27	0.02	792.09	846.17	99.74	402
1.37	0.02	1.28	1.06	0.16	402

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.29	0.02	554155.56	308874.16	100.00	402

Ret. Time: 1.29

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

