


3 CPK2017-720-00615

Catalog No:HY-10008 Batch#00615

Sample Name:	CPK2017-720-00615	Injection Volume:	5.0
Vial Number:	RA4	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	220
Control Program:	10-80A,220NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2017-7-21 10:22	Sample Weight:	1.0000
Run Time (min):	17.00	Sample Amount:	1.0000

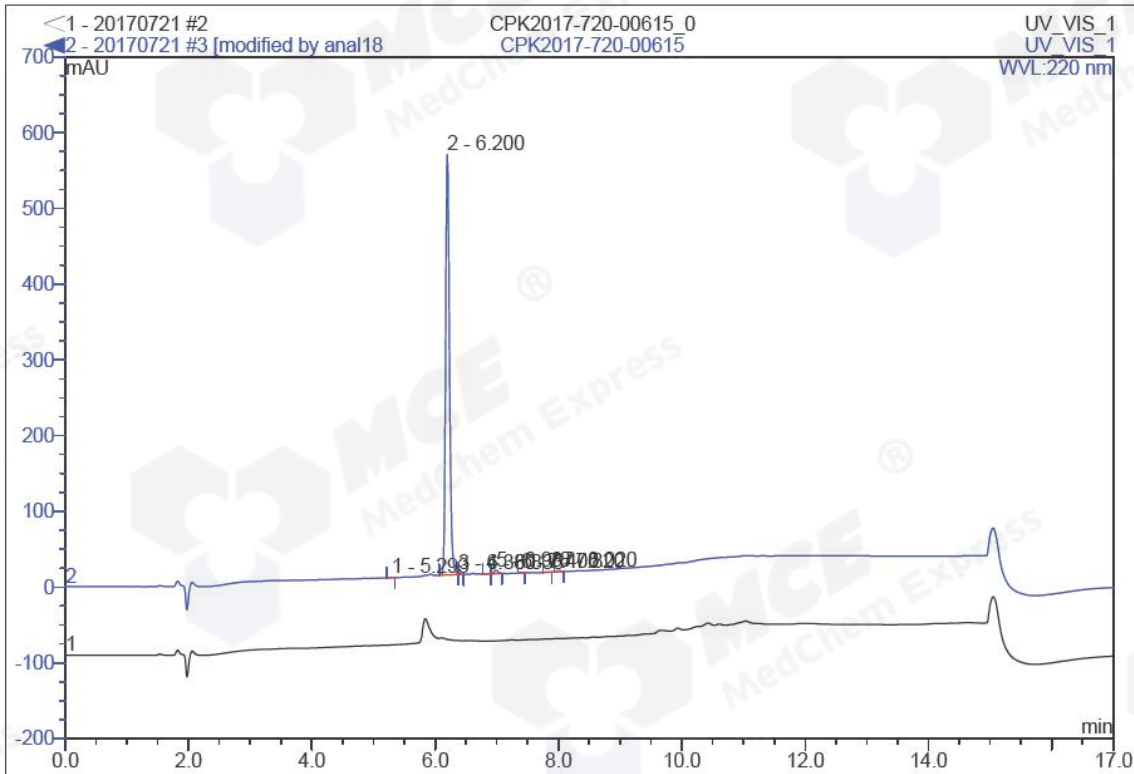

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	5.29	n.a.	0.521	0.032	0.08	n.a.	BMB*
2	6.20	n.a.	555.097	40.224	98.50	n.a.	BM *
3	6.38	n.a.	1.645	0.081	0.20	n.a.	MB*
4	6.83	n.a.	0.522	0.029	0.07	n.a.	BMB*
5	6.99	n.a.	4.567	0.320	0.78	n.a.	bMB*
6	7.40	n.a.	0.543	0.034	0.08	n.a.	BMB*
7	7.82	n.a.	0.390	0.030	0.07	n.a.	BMB*
8	8.02	n.a.	1.046	0.087	0.21	n.a.	BMB*
Total:			564.332	40.838	100.00	0.000	