



File ..\DATA\2020\20200828\1088\BIZ2020-827-SCH6.D Tgt Mass (CHM):  
Injection Date : 28 Aug 20 11:54 am +0800 Seq. Line : 44  
Sample Name : BIZ2020-827-SCH6 Location : P1-B-03  
Acq. Operator : zyj\_1547 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20200828\1088\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200828\1088\1-POS-3MIN.M  
Catalog No : HY-100155  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

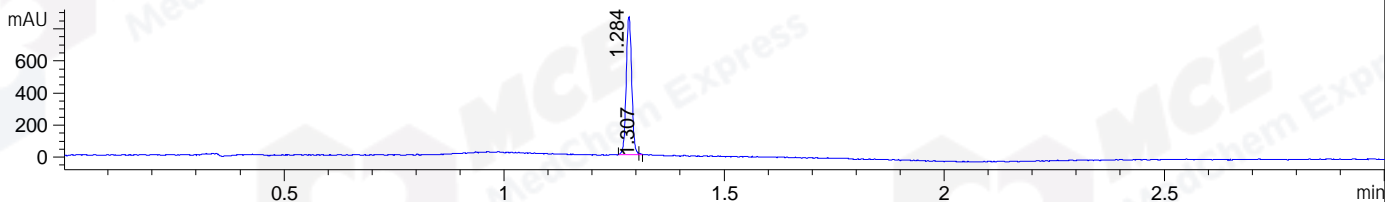


DAD1 C, Sig=254,4 Ref=off

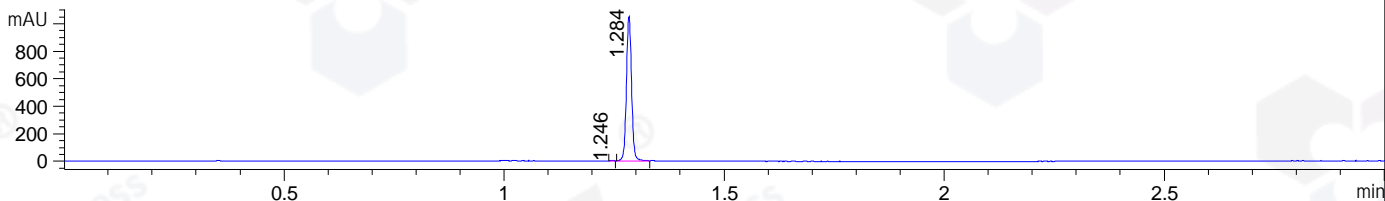

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

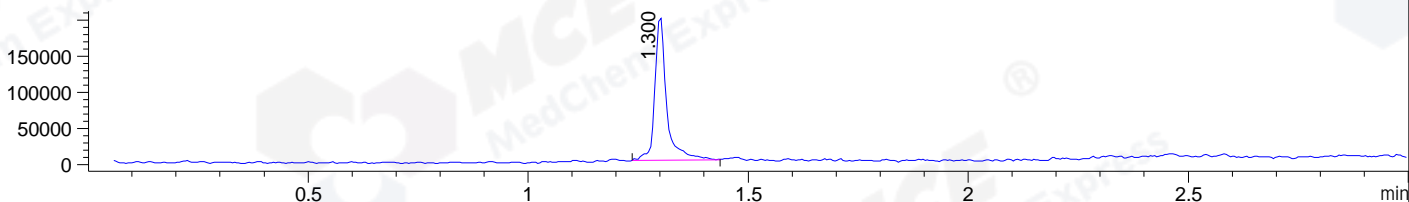

Ion 421, MSD1 421, Target Mass 420 +H Positive, EIC=420.7:421.7

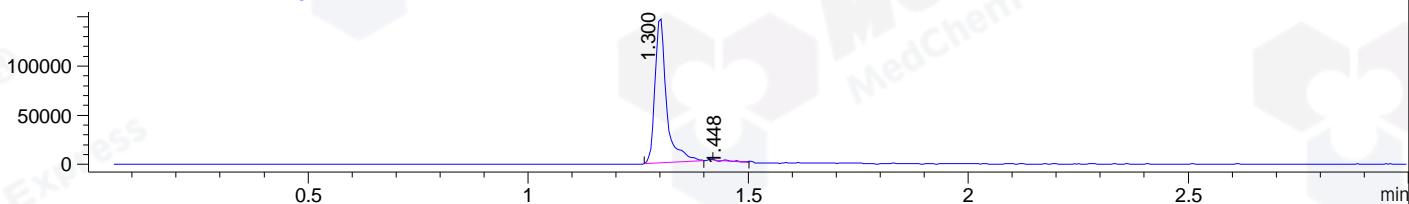

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.01	749.01	861.86	99.81	421
1.31	0.00	1.41	6.42	0.19	421

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.01	1.19	2.29	0.14	329
1.28	0.01	850.19	1051.78	99.86	421

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.30	0.03	372267.63	199309.48	100.00	421

Ret. Time: 1.30

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

