



File ..\DATA\2019\20190711\627\CPK2019-709-21377.D Tgt Mass (CHM):  
 Injection Date : 11 Jul 19 10:19 am +0800 Seq. Line : 20  
 Sample Name : CPK2019-709-21377 Location : P1-A-01  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2019\20190711\627\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2019\20190711\627\1-POS-3MIN.M  
 Catalog No : HY-100382 Batch#21377  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

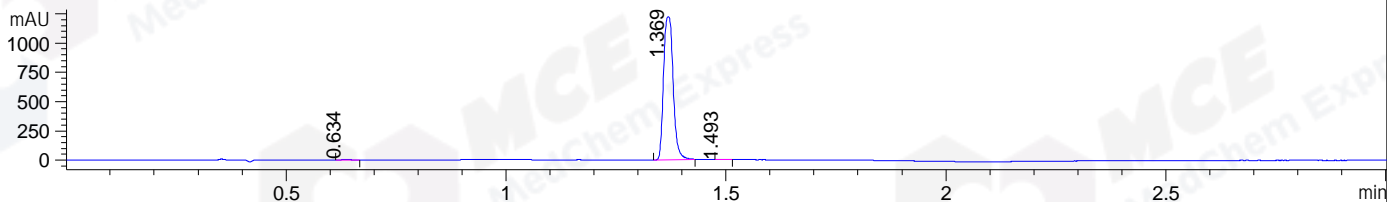


DAD1 C, Sig=254,4 Ref=off

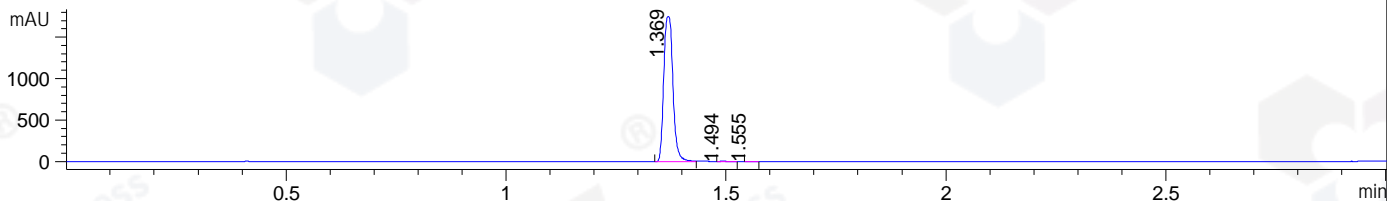

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

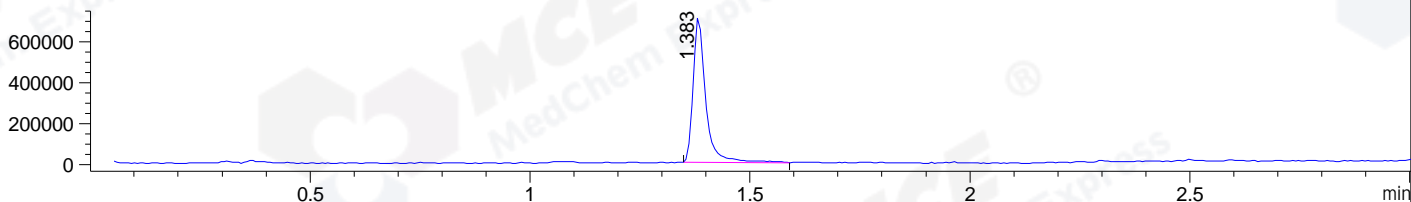

Ion 306.3171, MSD1 306.3171, Target Mass 305.3171 +H Positive, EIC=306.02:307.02

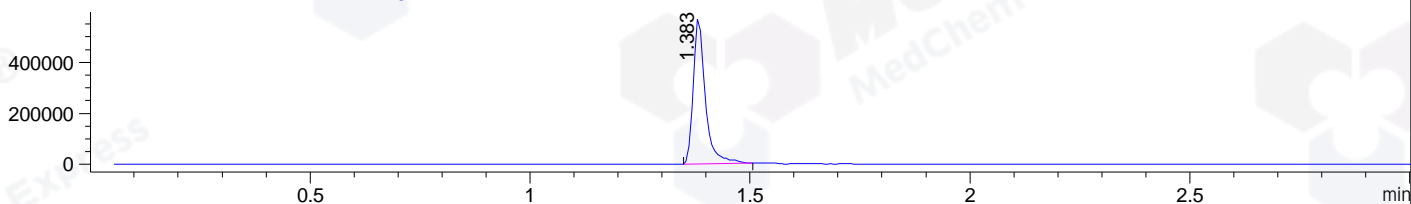

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.63	0.02	8.99	6.40	0.48	ND
1.37	0.02	1852.54	1223.74	99.42	306
1.49	0.02	1.84	1.89	0.10	306

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.37	0.02	2533.45	1751.06	99.91	306
1.49	0.02	1.66	1.81	0.07	306
1.56	0.01	0.64	0.75	0.03	306

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.03	1435334.63	710065.63	100.00	306

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

