

File ..\DATA\2019\20190615\590\CPK2019-612-21371.D Tgt Mass (CHM):

Injection Date : 15 Jun 19 9:57 am +0800 Seq. Line : 15

Sample Name : CPK2019-612-21371 Location : P2-A-02

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190615\590\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190615\590\1-POS-3MIN.M

Catalog No : HY-100403 Batch#21371

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

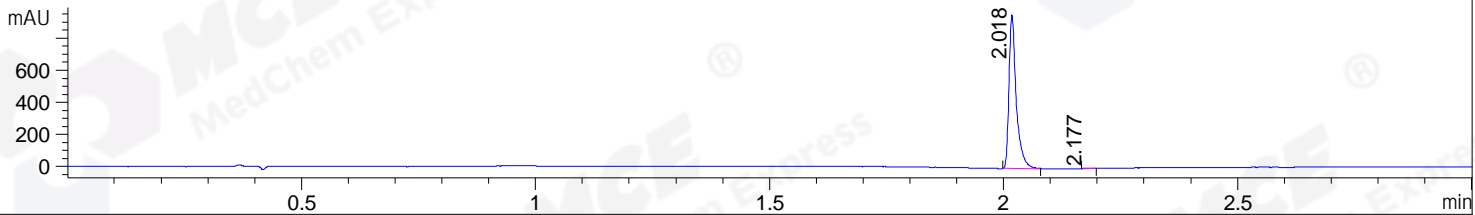


DAD1 C, Sig=254,4 Ref=off

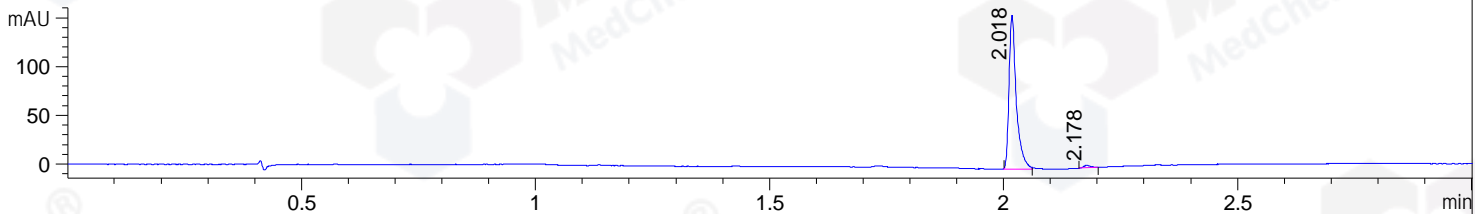

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

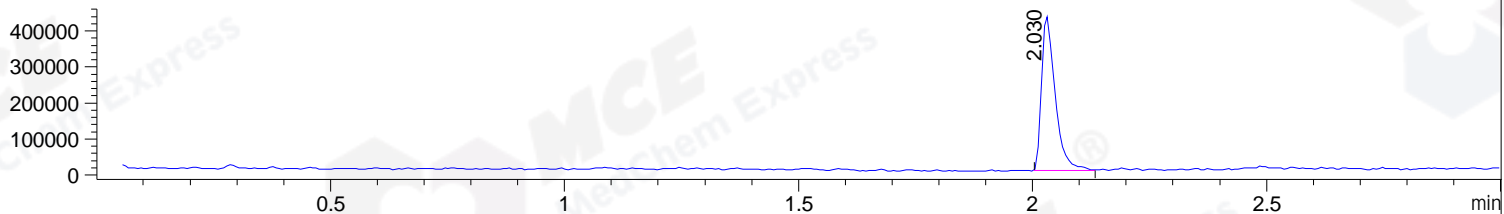

Ion 320.4009, MSD1 320.4009, Target Mass 319.4009 +H Positive, EIC=320.10:321.10

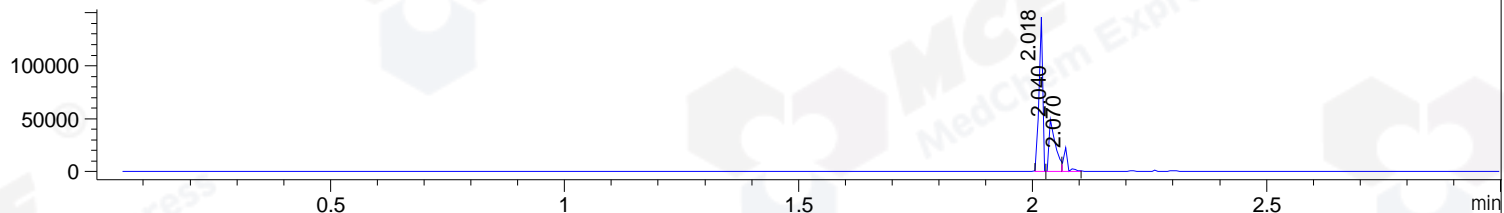

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.02	0.02	1030.06	958.06	99.80	320
2.18	0.01	2.10	2.33	0.20	134

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.02	0.02	169.07	157.92	98.57	320
2.18	0.02	2.45	2.44	1.43	134

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.03	0.03	877726.75	430403.13	100.00	320

Ret. Time: 2.03

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

