


File ..DATA\2019\20190508\576\CPK2019-506-22161-.D Tgt Mass (CHM):
 Injection Date : 8 May 19 5:39 pm +0800 Seq. Line : 23
 Sample Name : CPK2019-506-22161 Location : P1-A-07
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 2 ul
 Acq. Method : D:\Chem32\1\data\2019\20190508\576\1-POS-3MIN-1.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190508\576\1-POS-3MIN-1.M
 Catalog No : HY-100406 Batch# 22161 H2O+ACN
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-322
 Oven Temperature : 45□

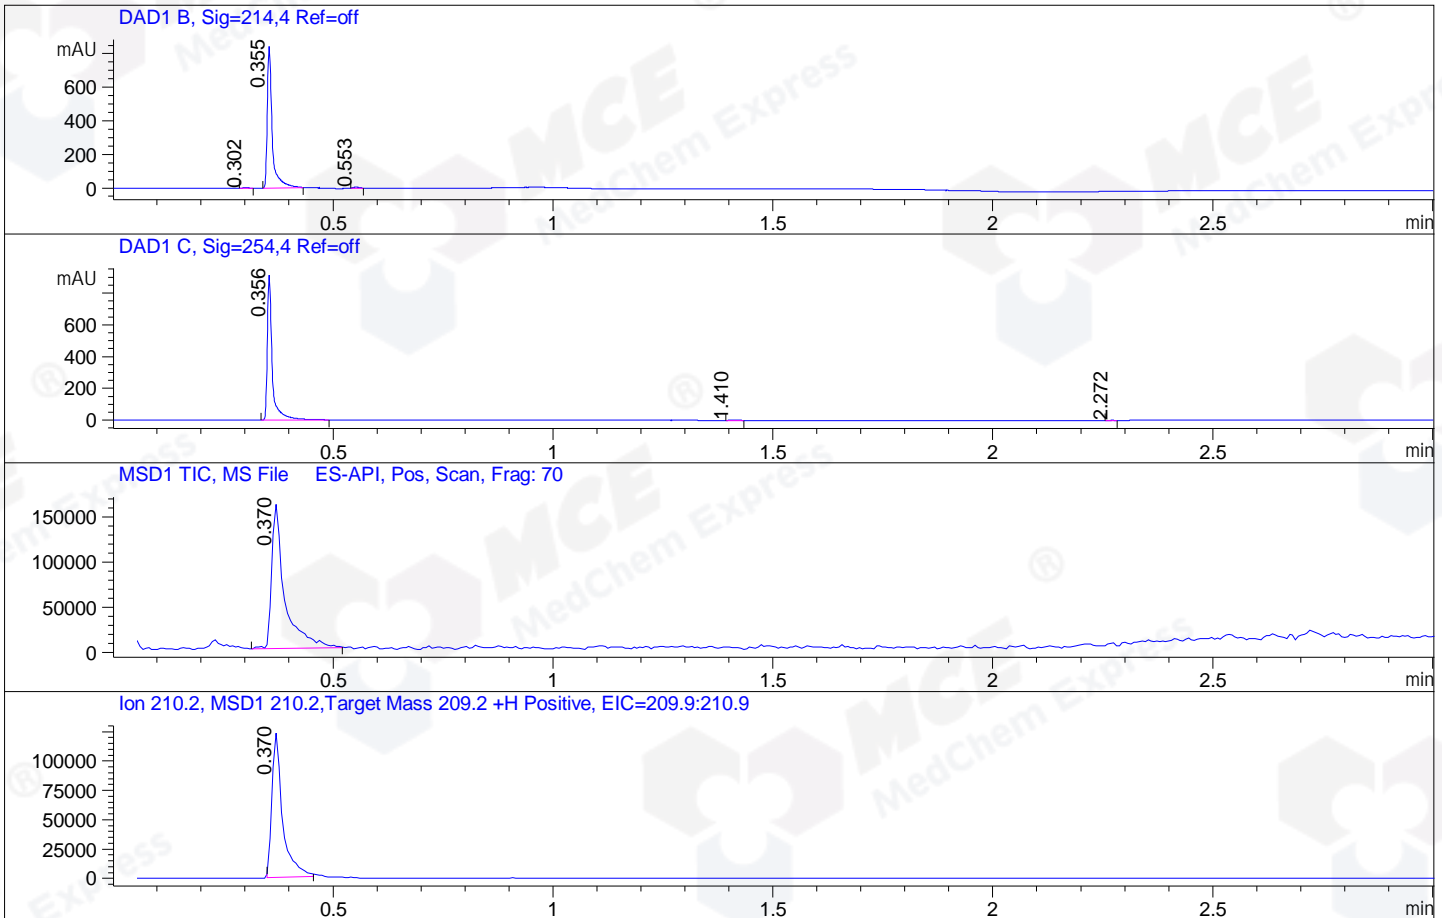

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.30	0.02	2.74	2.64	0.41	ND
0.36	0.01	665.96	897.61	98.80	210
0.55	0.01	5.36	6.29	0.80	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.36	0.01	715.42	857.59	99.59	210
1.41	0.02	2.45	2.39	0.34	ND
2.27	0.02	0.49	0.49	0.07	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
0.37	0.03	335071.06	160575.00	100.00	210

Ret. Time: 0.37

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

