



File ..\DATA\2020\20201026\1136\BIZ2020-O23-SCH1.D Tgt Mass (CHM):
 Injection Date : 26 Oct 20 7:02 pm +0800 Seq. Line : 101
 Sample Name : BIZ2020-O23-SCH1 Location : P1-D-08
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20201026\1136\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201026\1136\1-POS-3MIN.M
 Catalog No : HY-100545
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

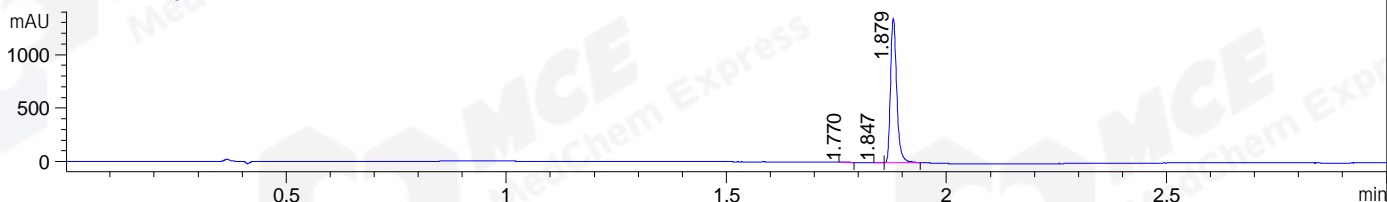


DAD1 C, Sig=254,4 Ref=off

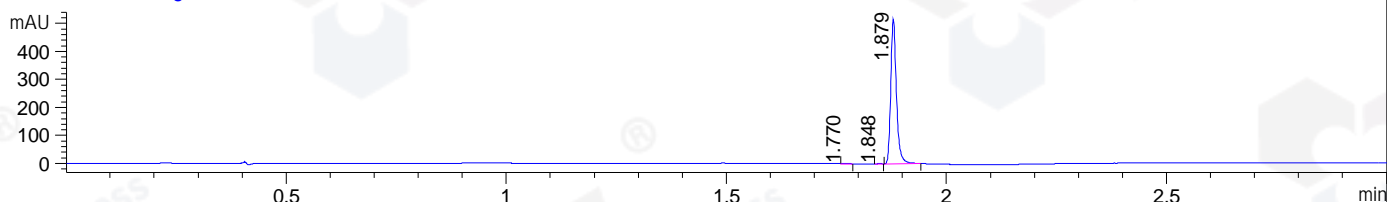

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

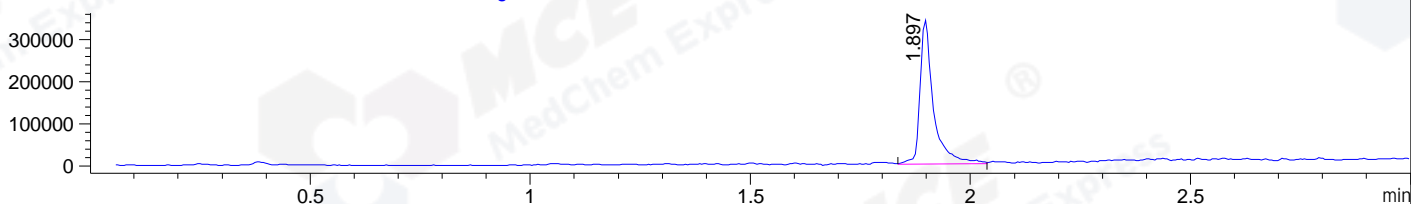

Ion 765, MSD1 765, Target Mass 764 +H Positive, EIC=764.7:765.7

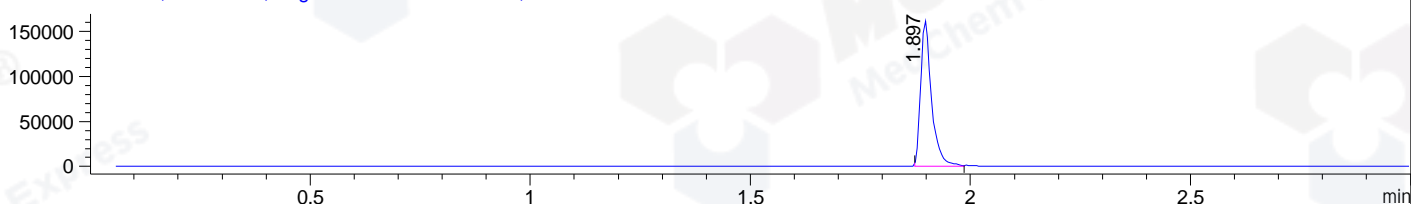

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.77	0.02	2.71	2.60	0.20	ND
1.85	0.01	2.38	3.26	0.18	ND
1.88	0.02	1323.18	1349.95	99.62	765

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.77	0.02	0.64	0.71	0.14	ND
1.85	0.01	0.61	0.92	0.13	ND
1.88	0.01	462.59	516.64	99.73	765

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.90	0.03	730497.69	341810.84	100.00	765

Ret. Time: 1.90

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

