



File ..\DATA\2019\20190917\719\CPK2019-912-23135.D Tgt Mass (CHM):
 Injection Date : 17 Sep 19 10:59 am +0800 Seq. Line : 22
 Sample Name : CPK2019-912-23135 Location : P1-B-04
 Acq. Operator : bgd_1571 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\Chem32\1\data\2019\20190917\719\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190917\719\1-POS-3MIN.M
 Catalog No : HY-100565 Batch#23135
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

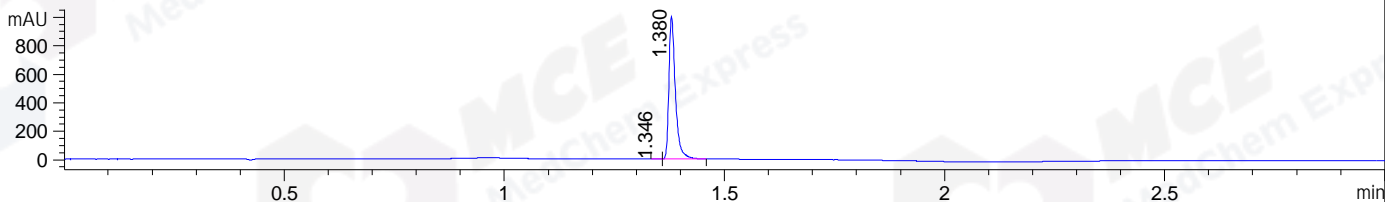


DAD1 C, Sig=254,4 Ref=off

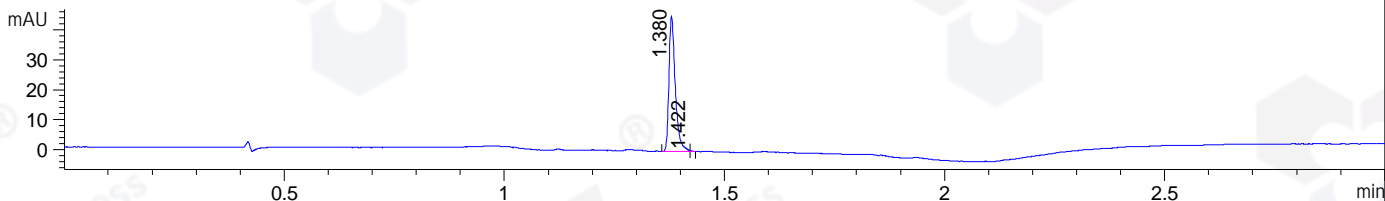

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

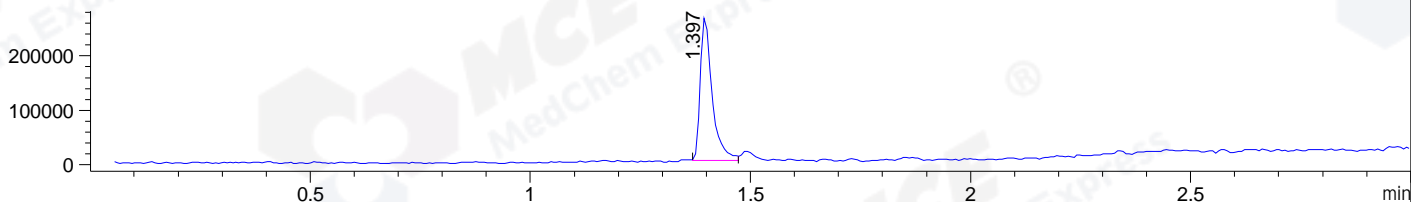

Ion 313.4153, MSD1 313.4153, Target Mass 312.4153 +H Positive, EIC=313.12:314.12

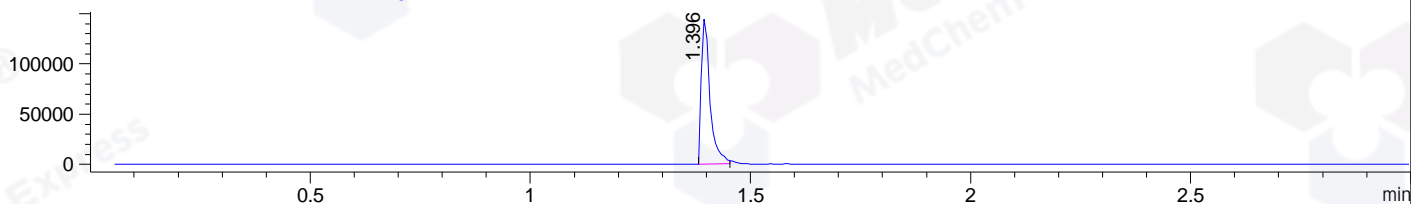

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.01	1.35	1.51	0.13	ND
1.38	0.02	1014.56	1001.69	99.87	313

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.02	44.74	45.10	99.87	313
1.42	0.00	0.06	0.24	0.13	313

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.40	0.03	495590.25	266201.59	100.00	313

Ret. Time: 1.40

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

