



File ..\DATA\2019\20190716\630\CPK2019-715-22366.D Tgt Mass (CHM):
 Injection Date : 16 Jul 19 2:50 pm +0800 Seq. Line : 75
 Sample Name : CPK2019-715-22366 Location : PI-A-07
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190716\630\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190716\630\1-POS-3MIN.M
 Catalog No : HY-100746 Batch#22366
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45


DAD1 C, Sig=254,4 Ref=off

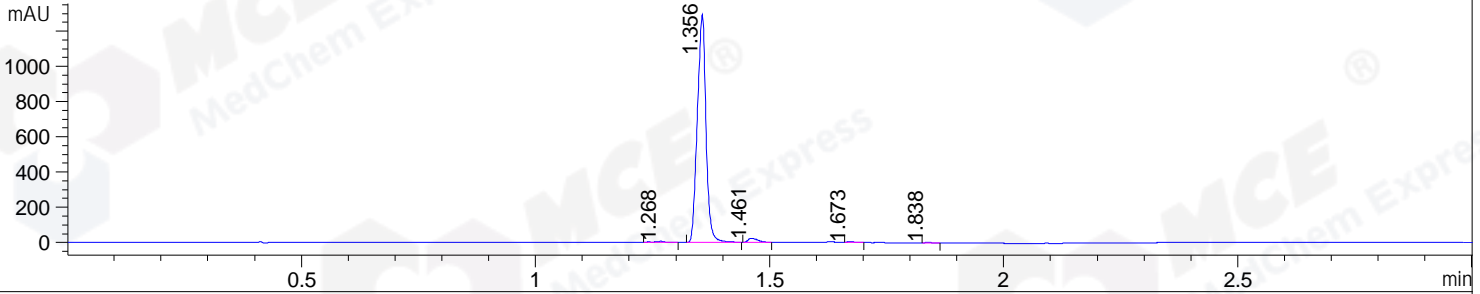

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

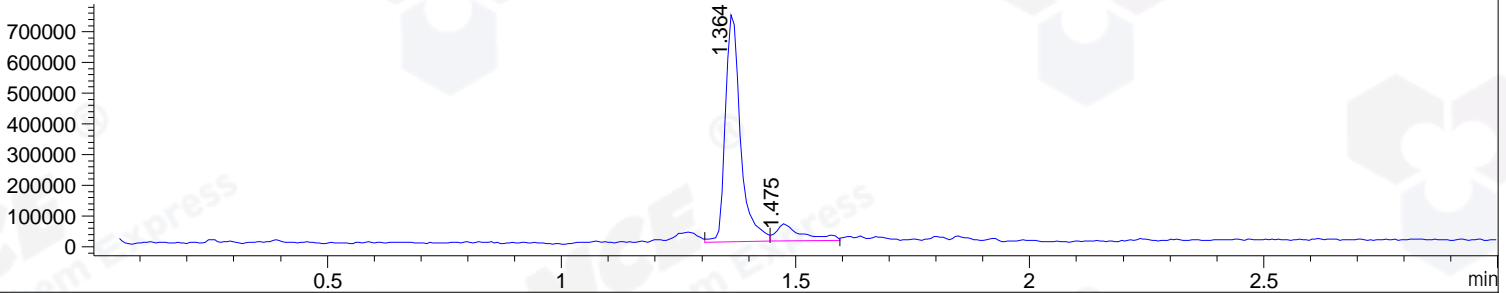

Ion 268.355, MSD1 268.355, Target Mass 267.355 +H Positive, EIC=268.06:269.06

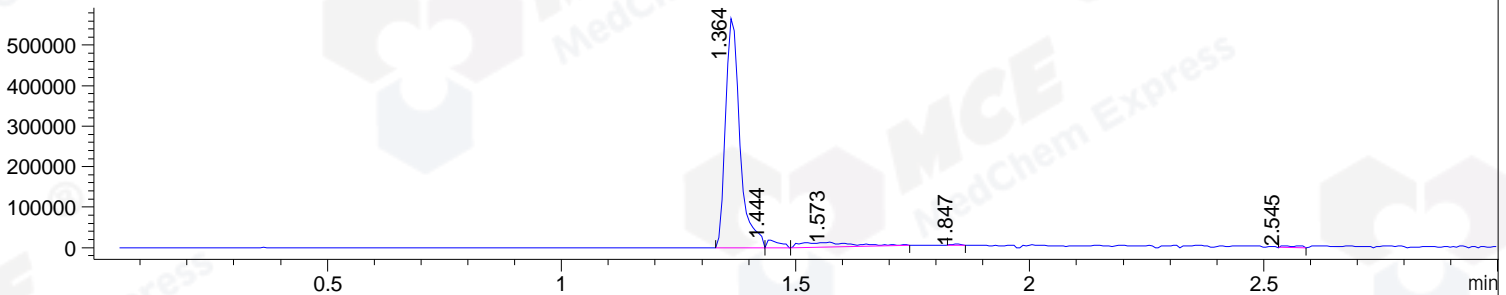

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.27	0.02	9.96	6.95	0.58	387
1.36	0.02	1668.88	1293.88	97.20	268
1.46	0.02	31.53	22.04	1.84	268
1.67	0.02	4.22	4.14	0.25	268
1.84	0.02	2.33	2.32	0.14	268

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.03	1661034.13	746112.88	88.16	268
1.47	0.05	223067.94	57735.25	11.84	268

Ret. Time: 1.36

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.47

ES-API Positive

