



File ..\DATA\2019\20190720\650\CPK2019-717-22379.D Tgt Mass (CHM):
Injection Date : 20 Jul 19 11:59 am +0800 Seq. Line : 41
Sample Name : CPK2019-717-22379 Location : P1-D-03
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190720\650\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190720\650\1-POS-3MIN.M
Catalog No : HY-100769 Batch#22379
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

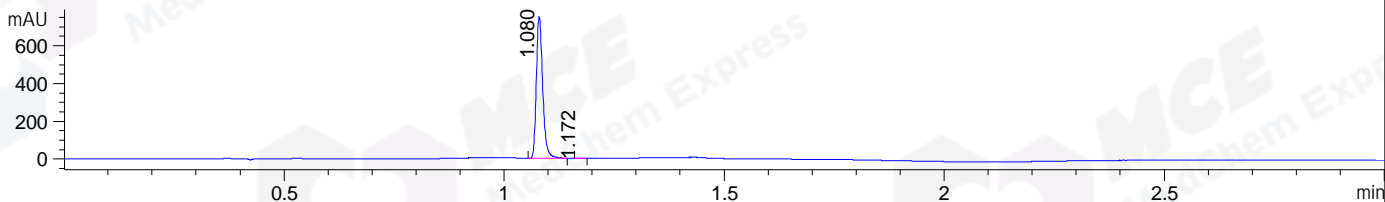


DAD1 C, Sig=254,4 Ref=off

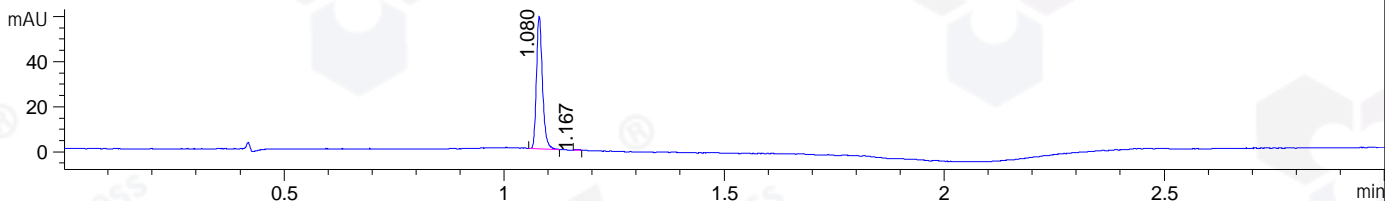

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

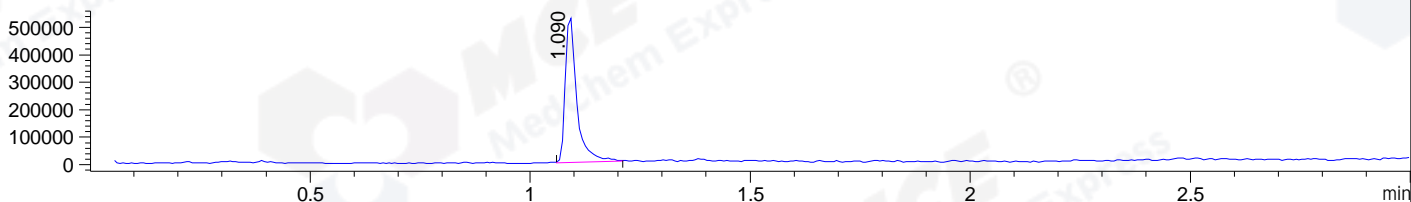

Ion 335.8492, MSD1 335.8492, Target Mass 334.8492 +H Positive, EIC=335.55:336.55

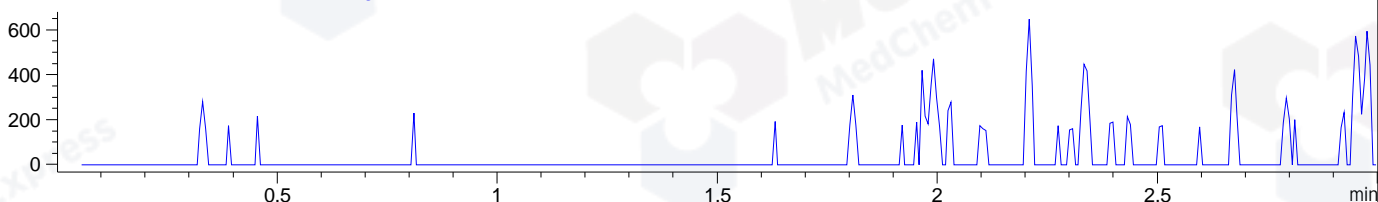

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.02	751.24	750.71	99.77	299
1.17	0.02	1.74	1.72	0.23	299

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.02	55.27	58.78	99.70	299
1.17	0.01	0.17	0.22	0.30	299

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.02	958046.44	536611.50	100.00	299

Ret. Time: 1.09

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

