
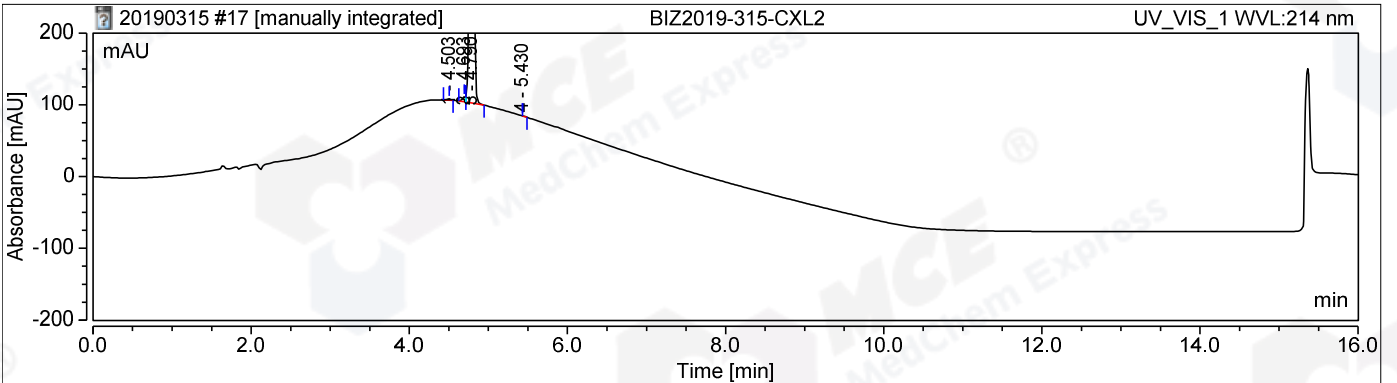


Chromatogram and Results

Injection Details

Injection Name: BIZ2019-315-CXL2	Run Time (min): 16.00
Vial Number: RC6	Users: zqq
Injection Type: Unknown	Injection Volume: 5.00
Calibration Level:	Channel: UV_VIS_1
Instrument Method: 10-90A 214NM	Wavelength: 214
Processing Method: New processing	Bandwidth: 4
Catalog No: HY-100962 Batch#39004-20190315 A-RP-328	Dilution Factor: 1.0000
Injection Date/Time: 15/Mar/19 17:35	Sample Weight: 1.0000

Chromatogram

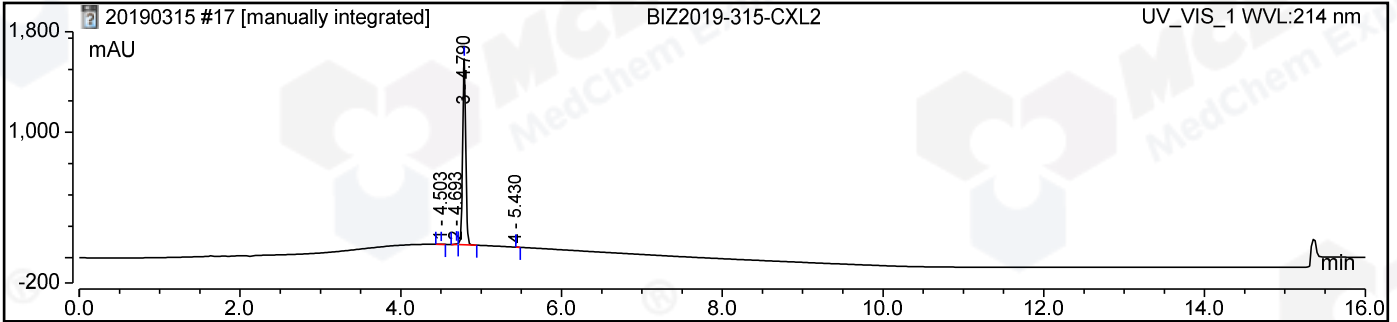

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
1		4.503	0.085	1.756	n.a.	988	0.91	0.13
2		4.693	0.304	6.702	n.a.	970	n.a.	0.45
3		4.790	67.179	1481.967	n.a.	999	0.99	99.41
4		5.430	0.011	0.000	n.a.	0	n.a.	0.02
Total:			67.581	1490.425	0.00			1.90