
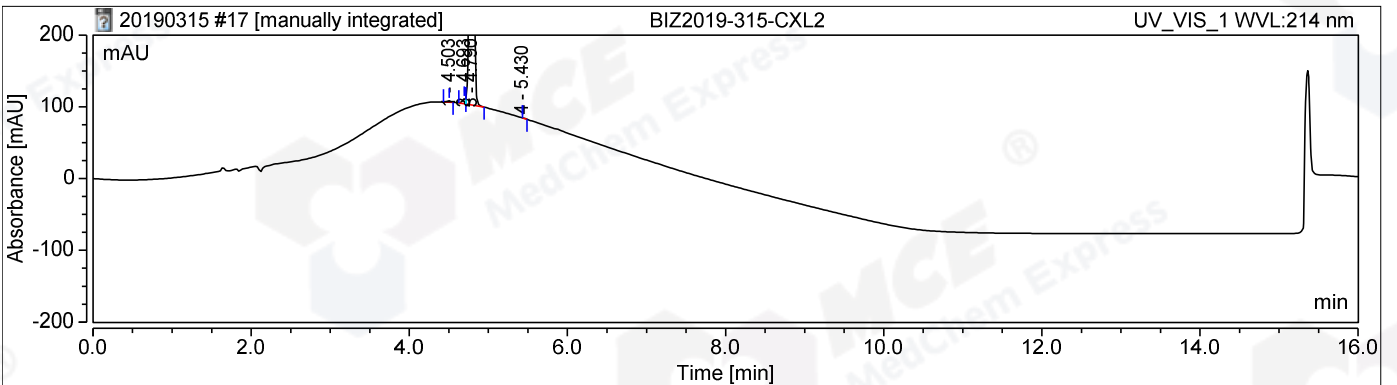


### Chromatogram and Results

#### Injection Details

Injection Name: <b>BIZ2019-315-CXL2</b>	Run Time (min): <b>16.00</b>
Vial Number: <b>RC6</b>	Users: <b>zqq</b>
Injection Type: <b>Unknown</b>	Injection Volume: <b>5.00</b>
Calibration Level:	Channel: <b>UV_VIS_1</b>
Instrument Method: <b>10-90A 214NM</b>	Wavelength: <b>214</b>
Processing Method: <b>New processing</b>	Bandwidth: <b>4</b>
Catalog No: <b>HY-100962 Batch#39004-20190315 A-RP-328</b>	Dilution Factor: <b>1.0000</b>
Injection Date/Time: <b>15/Mar/19 17:35</b>	Sample Weight: <b>1.0000</b>

#### Chromatogram

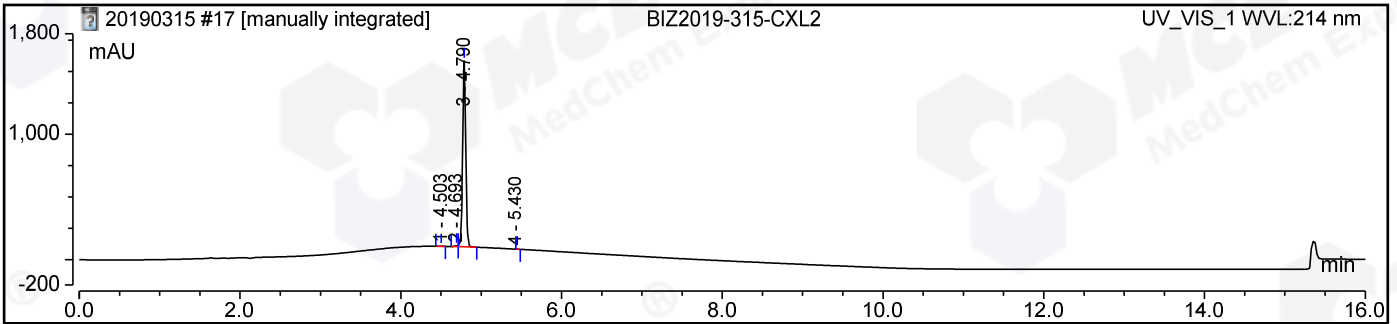

#### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
1		4.503	0.085	1.756	n.a.	988	0.91	0.13
2		4.693	0.304	6.702	n.a.	970	n.a.	0.45
3		4.790	67.179	1481.967	n.a.	999	0.99	99.41
4		5.430	0.011	0.000	n.a.	0	n.a.	0.02
Total:			67.581	1490.425	0.00			1.90