


Chromatogram and Results

Injection Details

Injection Name: BLANK	Injection Volume: 5.00
Vial Number: BC1	Channel: UV_VIS_1
Injection Type: Unknown	Wavelength: 220
Calibration Level:	Users: jlw
Instrument Method: 5-80A.M	Dilution Factor: 1.0000
Processing Method: New Processing Method	Sample Weight: 1.0000
Injection Date/Time: 21/Jul/20 10:26	Run Time (min): 16.00
Comment: BLANK A-RP-538	

chrom://hy261/Thermo/Instrument Data/202007/20200721.seq/916.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

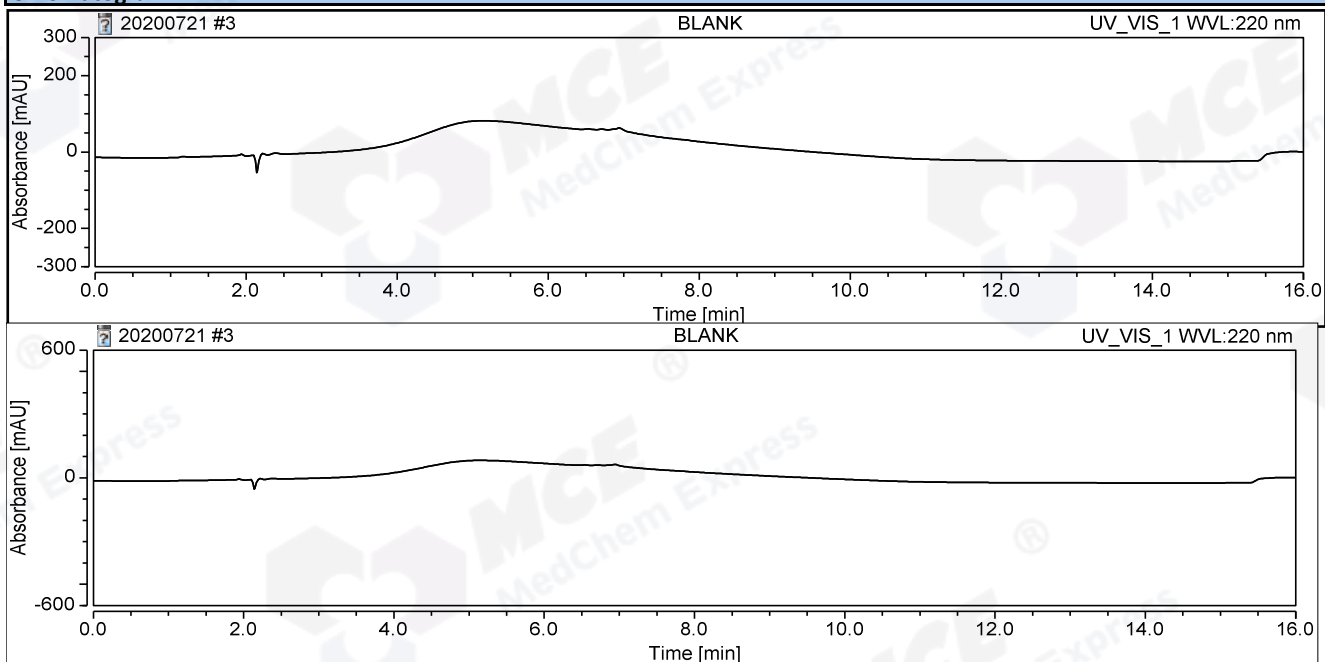

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	S/N	Rel.Area %
Total:			0.000	0.000	0.00	0.00	


Chromatogram and Results

Injection Details

Injection Name: CPK2020-720-03270	Injection Volume: 2.00
Vial Number: BC2	Channel: UV_VIS_1
Injection Type: Unknown	Wavelength: 220
Calibration Level:	Users: jlw
Instrument Method: 5-80A.M	Dilution Factor: 1.0000
Processing Method: New Processing Method	Sample Weight: 1.0000
Injection Date/Time: 21/Jul/20 10:44	Run Time (min): 16.00
Comment: HM-069_9-20171117 A-RP-538	

chrom://hy261/Themo/Instrument Data/202007/20200721.seq/636.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

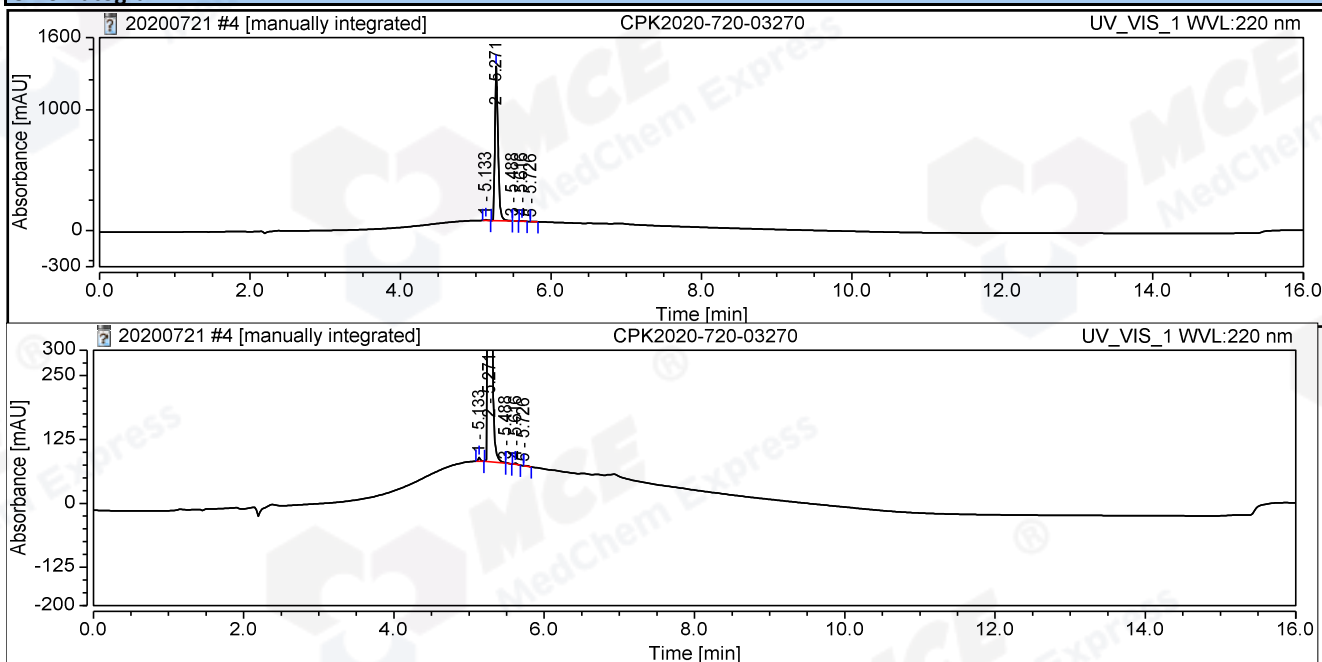

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	S/N	Rel.Area %
1		5.133	0.255	7.486	1.26	4.0	0.41
2		5.271	61.601	1279.189	1.48	683.9	99.27
3		5.488	0.048	0.997	n.a.	0.5	0.08
4		5.616	0.115	3.162	1.22	1.7	0.19
5		5.726	0.033	0.000	n.a.	0.0	0.05
Total:			62.053	1290.833	3.96	690.14	