


19 BIZ2019-D04-SCH2**Catalog No: HY-101402A Batch#59876 A-RP-243 JLW**

Sample Name:	BIZ2019-D04-SCH2	Injection Volume:	5.0
Vial Number:	BE7	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-12-27 16:35	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

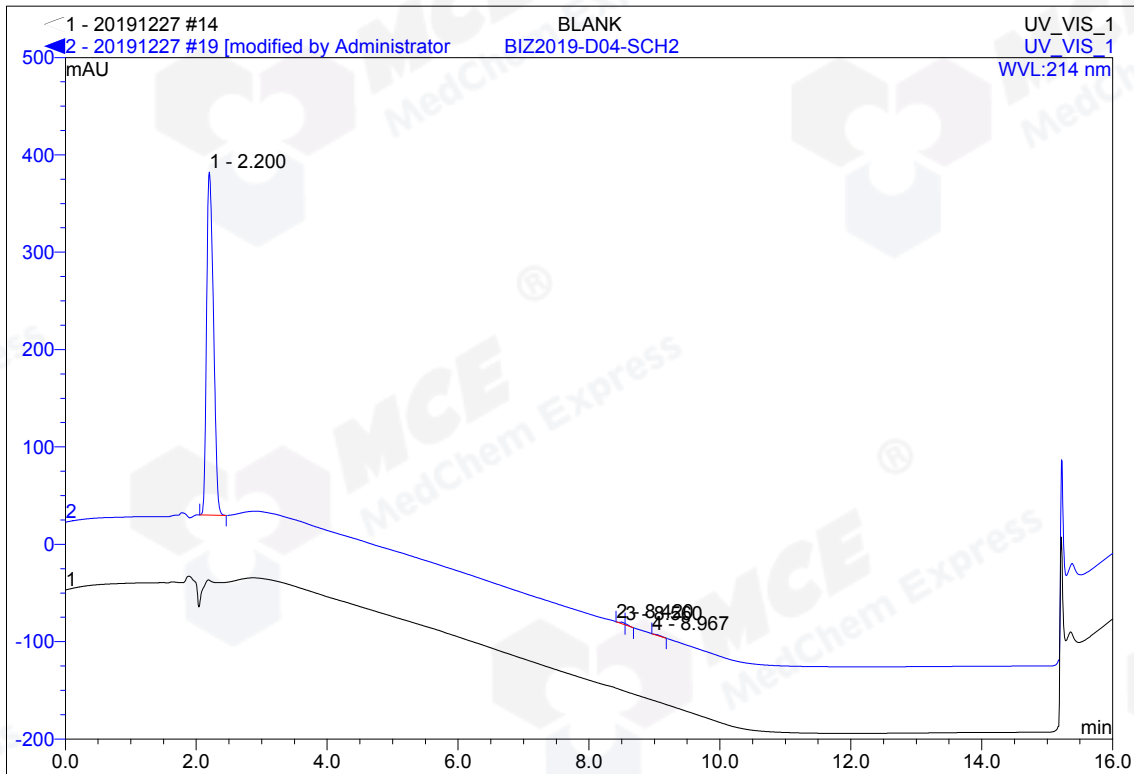

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	2.20	n.a.	352.542	42.812	99.35	n.a.	BMB*
2	8.42	n.a.	0.001	0.130	0.30	n.a.	BM
3	8.56	n.a.	1.237	0.079	0.18	n.a.	MB
4	8.97	n.a.	0.009	0.070	0.16	n.a.	BMB*
Total:			353.790	43.091	100.00	0.000	