



File ..DATA\2020\20200403\911\CPK2020-331-24639-.D Tgt Mass (CHM):  
 Injection Date : 3 Apr 20 9:01 am +0800 Seq. Line : 3  
 Sample Name : CPK2020-331-24639 Location : P1-C-07  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1.5 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200403\911\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200403\911\1-POS-3MIN.M  
 Catalog No : HY-101441A Batch#24639  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45


DAD1 C, Sig=254,4 Ref=off

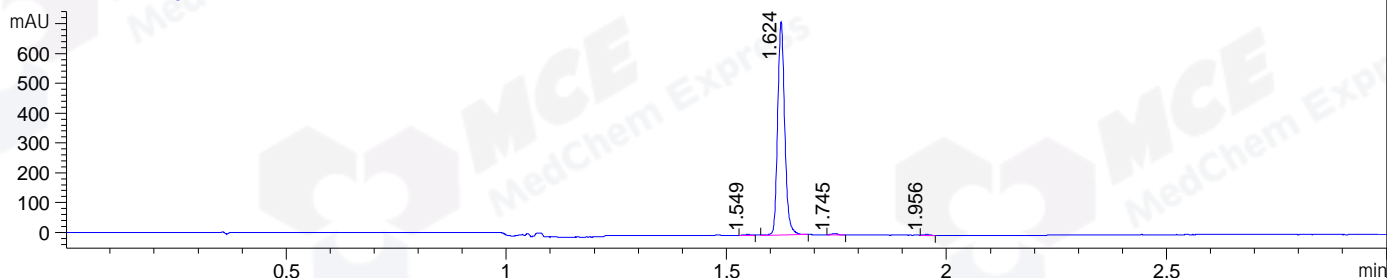

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

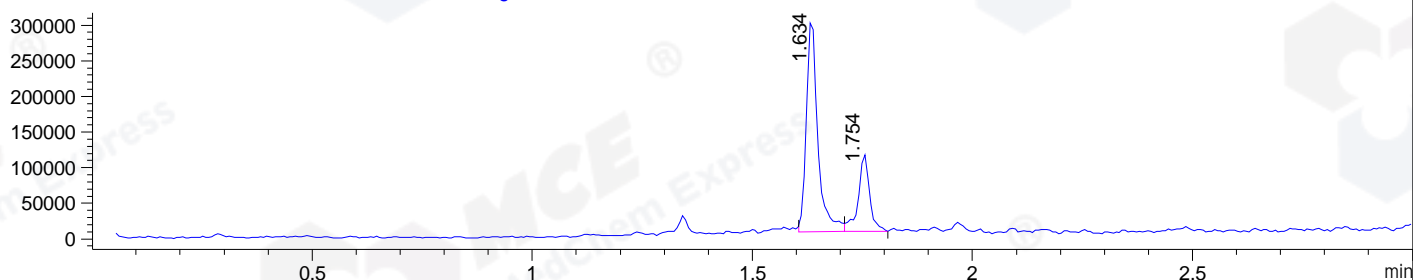

Ion 408, MSD1 408, Target Mass 407 +H Positive, EIC=407.7:408.7

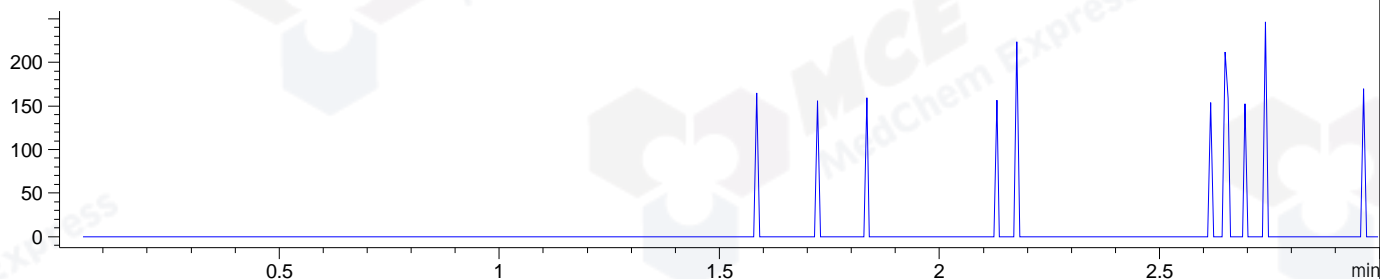

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.55	0.02	3.86	2.92	0.48	388
1.62	0.02	795.15	714.85	98.54	372
1.74	0.02	4.32	4.47	0.54	301
1.96	0.02	3.64	3.30	0.45	755


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.63	0.03	540415.56	302090.91	74.02	372
1.75	0.03	189638.66	108562.95	25.98	301

Ret. Time: 1.63

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

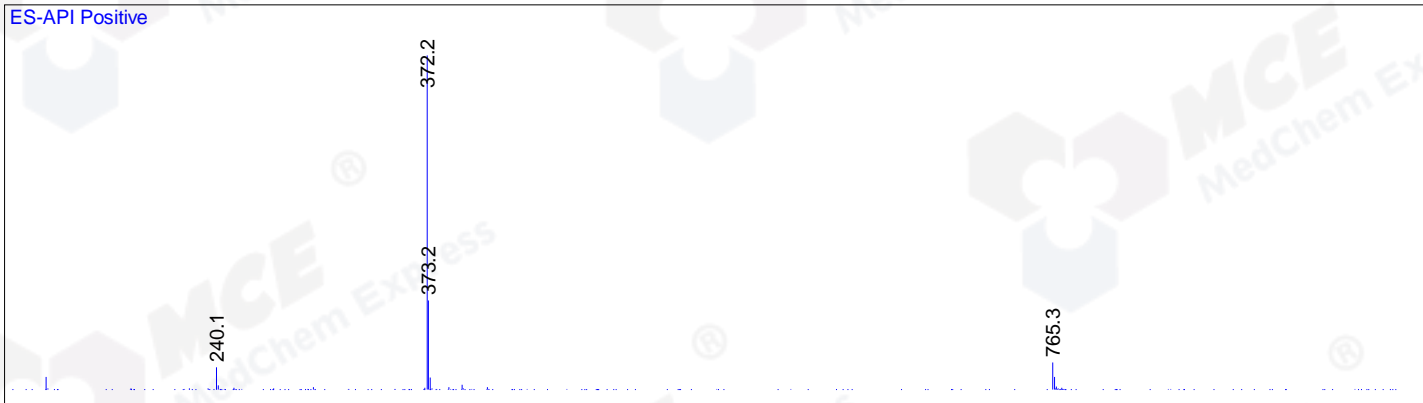

Ret. Time: 1.75

ES-API Positive

