

File ..DATA\2020\20200309\864\CPK2020-305-24564-.D Tgt Mass (CHM):

Injection Date : 9 Mar 20 1:24 pm +0800 Seq. Line : 56

Sample Name : CPK2020-305-24564 Location : P1-B-06

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 2 ul

Acq. Method : D:\Chem32\1\data\2020\20200309\864\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200309\864\1-POS-3MIN.M

Catalog No : HY-101464 Batch# 24564

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

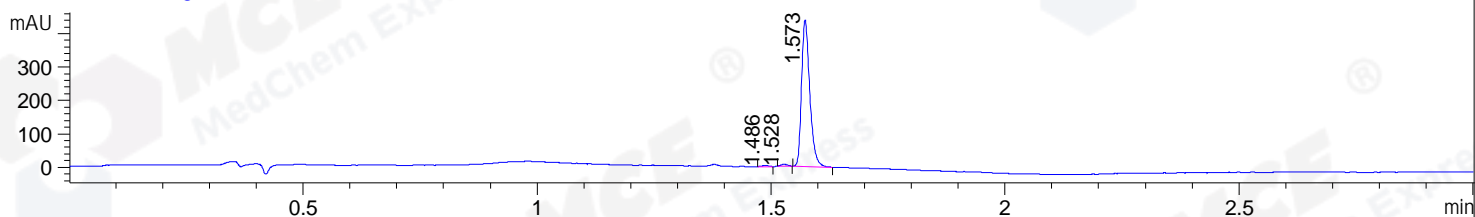


DAD1 C, Sig=254,4 Ref=off

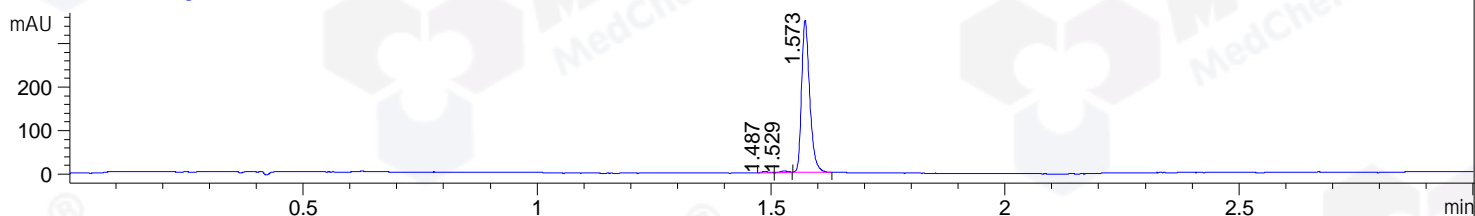

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

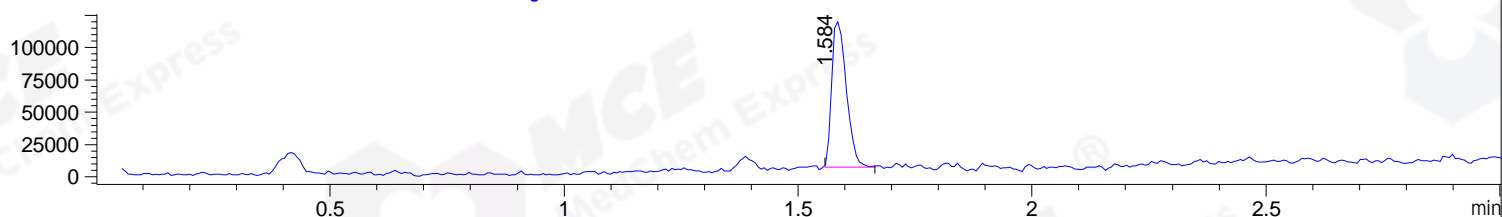

Ion 329, MSD1 329, Target Mass 328 +H Positive, EIC=328.7:329.7

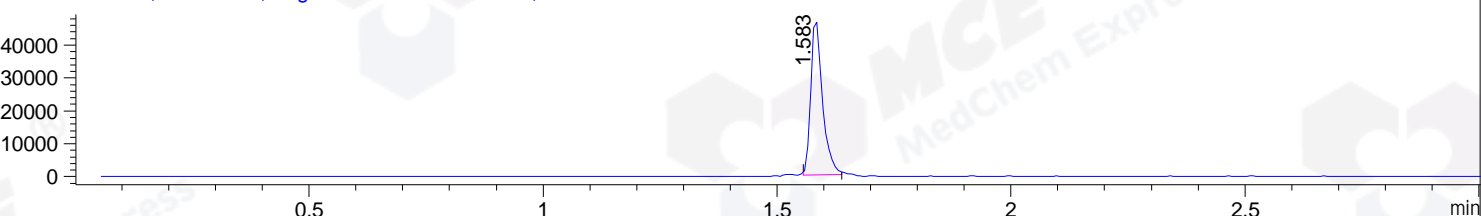

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.49	0.02	2.59	2.87	0.47	ND
1.53	0.02	5.26	5.44	0.96	ND
1.57	0.02	537.72	438.97	98.56	329

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.49	0.02	2.46	2.46	0.58	ND
1.53	0.01	2.94	2.87	0.69	ND
1.57	0.02	420.38	349.53	98.73	329

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.58	0.04	247547.53	112573.07	100.00	329

Ret. Time: 1.58

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

