



File ..1\DATA\2019\20190720\650\BIZ2019-719-WYQ1.D Tgt Mass (CHM):
 Injection Date : 20 Jul 19 10:32 am +0800 Seq. Line : 22
 Sample Name : BIZ2019-719-WYQ1 Location : P1-B-04
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190720\650\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190720\650\1-POS-3MIN.M
 Catalog No : HY-10167A Batch#43810
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

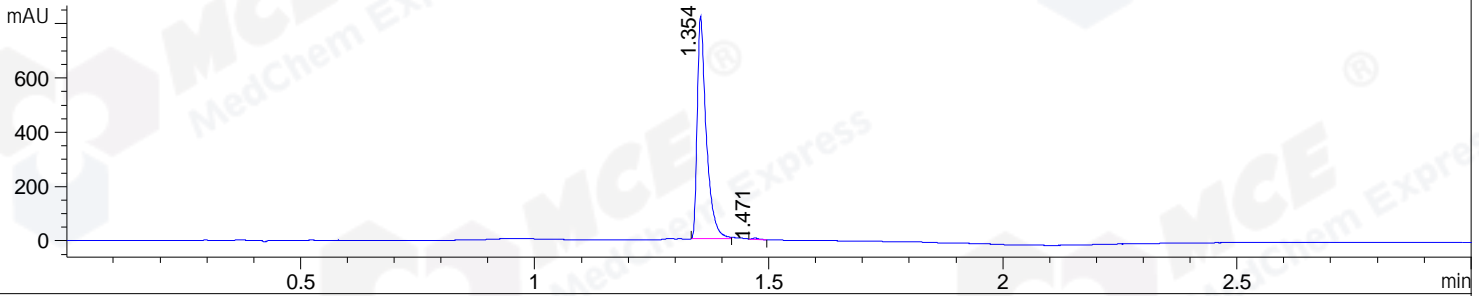

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

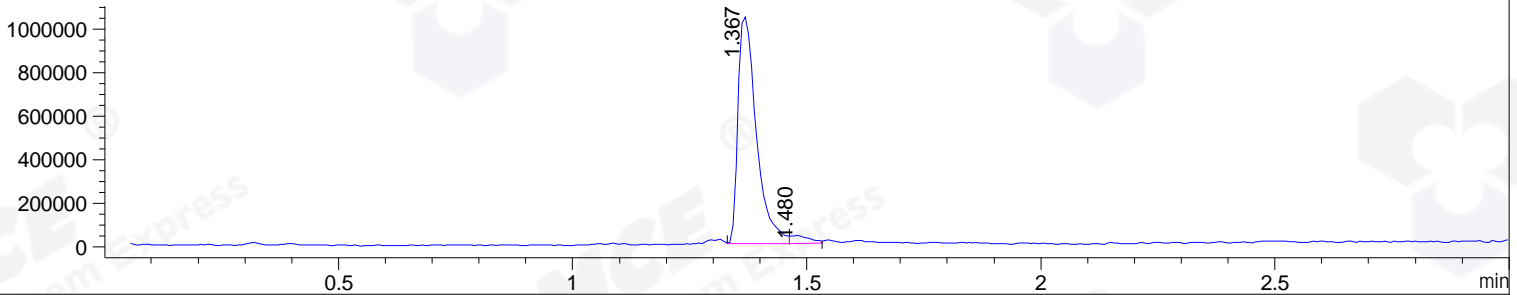

Ion 340.1, MSD1 340.1, Target Mass 339.1 +H Positive, EIC=339.8:340.8

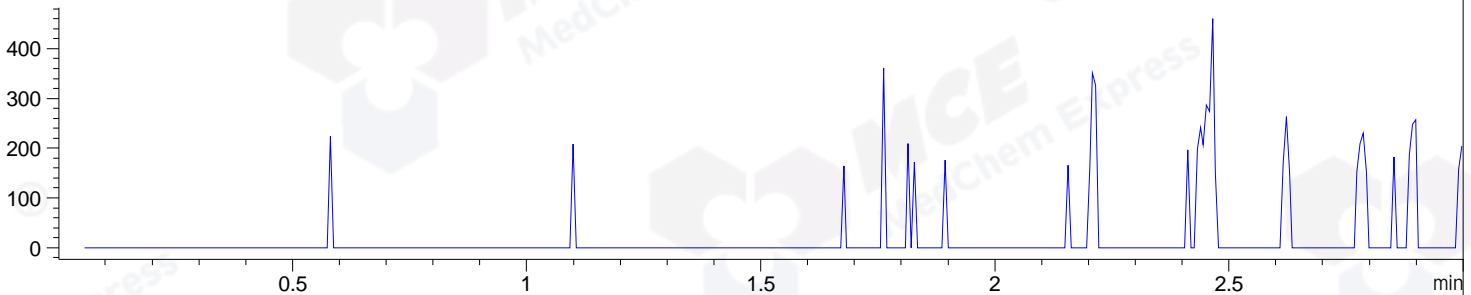

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.02	1099.46	818.31	99.66	304
1.47	0.01	3.71	4.28	0.34	304


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.37	0.04	2860891.50	1042047.19	96.58	304
1.48	0.04	101265.48	37618.98	3.42	304

Ret. Time: 1.37

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

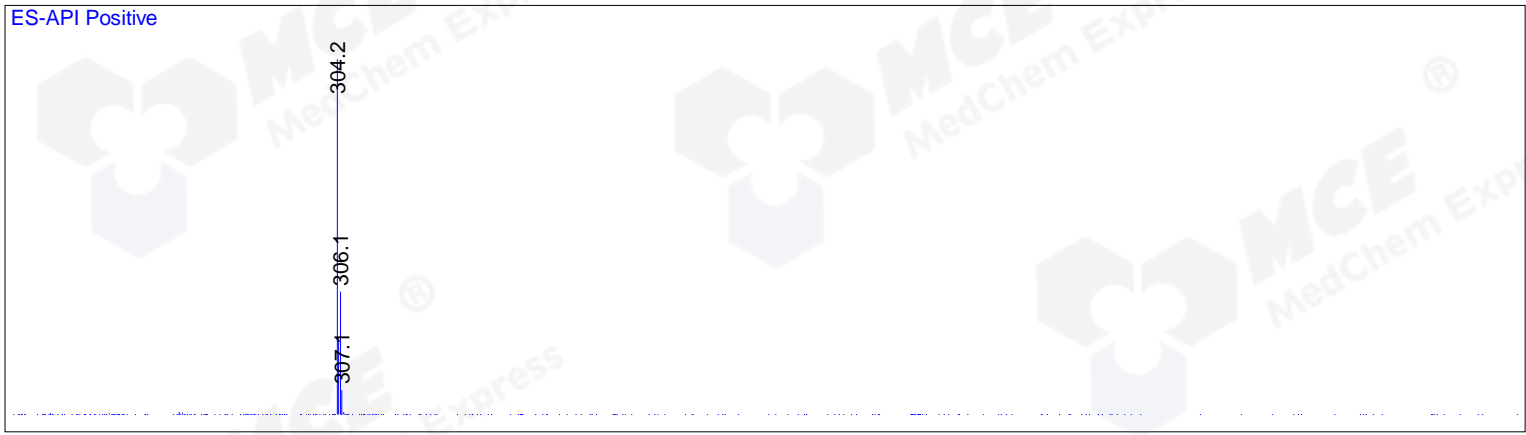

Ret. Time: 1.48

ES-API Positive

