
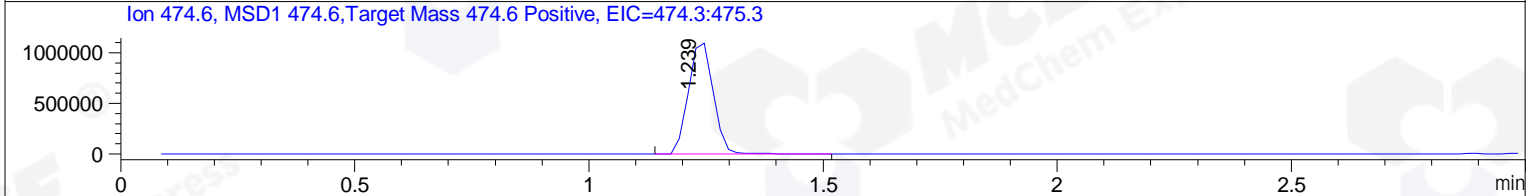
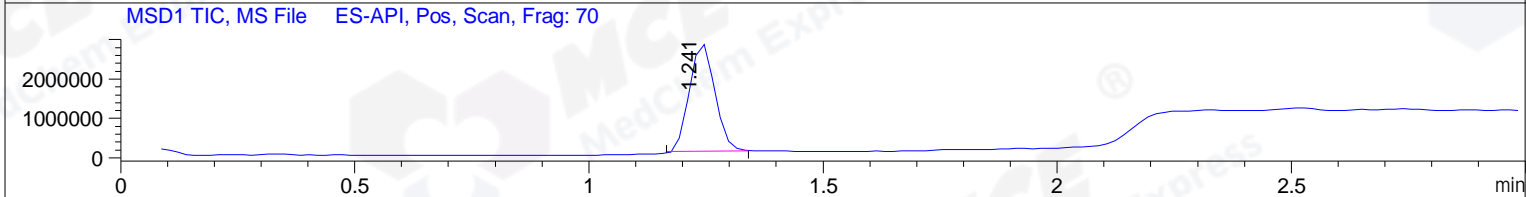
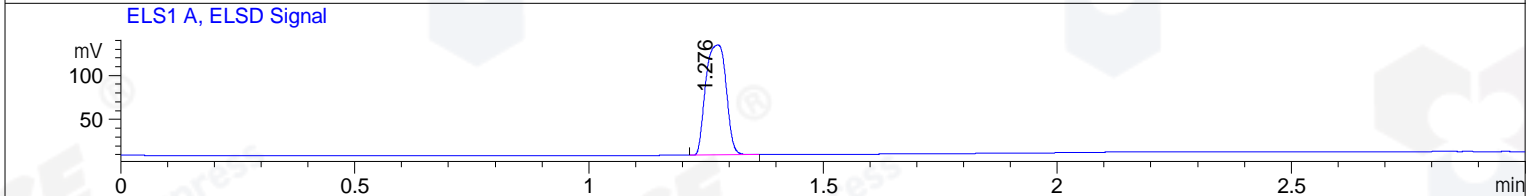
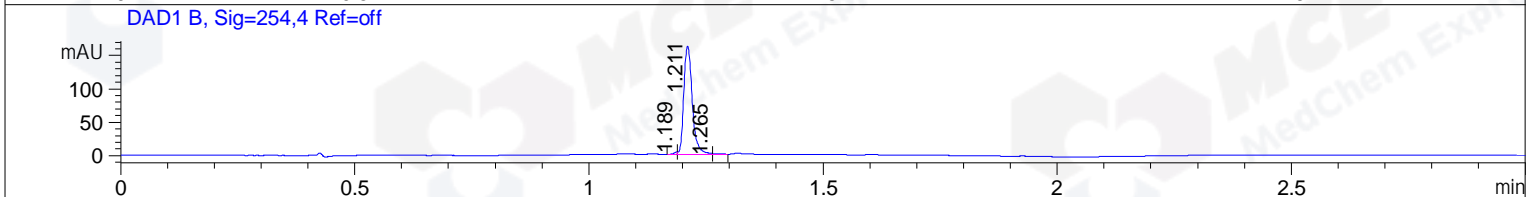


File ..ata\20170925\20170925 1\CPK2017-925-07899.D Tgt Mass (CHM):  
 Injection Date : 25 Sep 17 7:33 pm +0800 Seq. Line : 118  
 Sample Name : CPK2017-925-07899 Location : P2-A-11  
 Acq. Operator : SYSTEM Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\LCMS03\Data\20170925\20170925 1\1-POS-3MIN.M  
 Analysis Method : D:\LCMS03\Data\20170925\20170925 1\1-POS-3MIN.M  
 Catalog No : HY-10179 Batch#07899  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-186  
 Oven Temperature : 45C

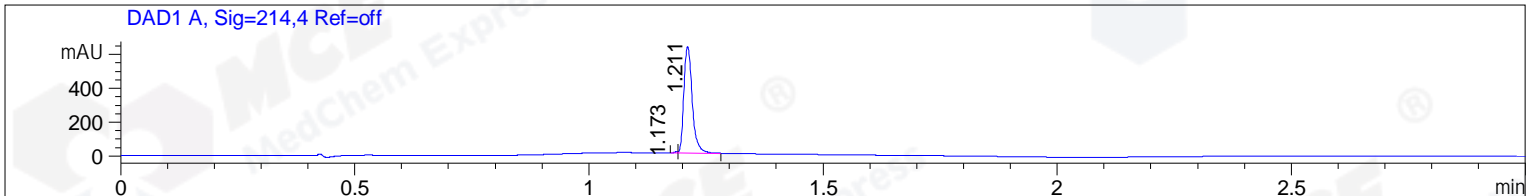

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.01	4.42	0.32	0.56	475
1.21	0.02	786.35	628.82	99.44	475

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%	MS (+)
1.19	0.01	1.68	3.64	0.81	475
1.21	0.02	203.62	161.94	98.77	475
1.26	0.01	0.86	1.01	0.42	475

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.06	10386308.00	2789096.75	100.00	475

Ret. Time: 1.24

<<<< POSITIVE SPECTRA >>>>

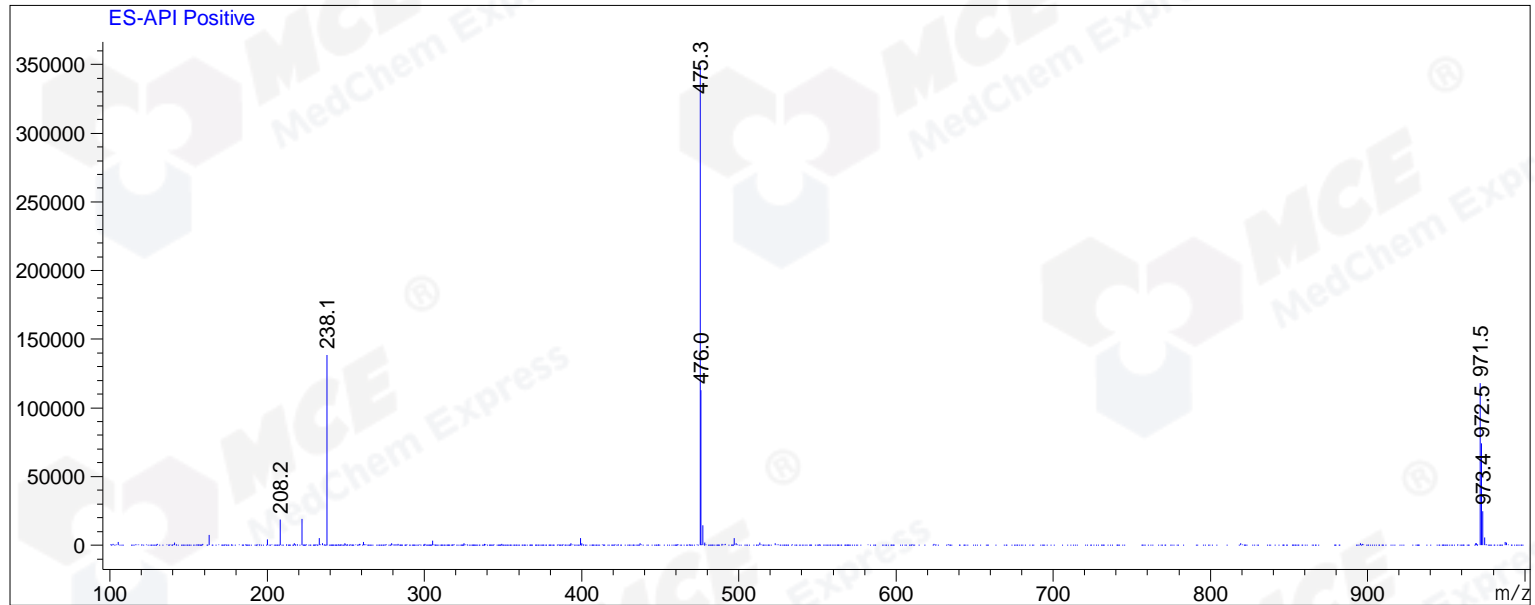

\*\*\* End of Report \*\*\*