



File ..\DATA\2020\20200328\898\CPK2020-324-03040.D Tgt Mass (CHM):  
 Injection Date : 28 Mar 20 4:54 pm +0800 Seq. Line : 91  
 Sample Name : CPK2020-324-03040 Location : P1-E-07  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200328\898\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200328\898\1-POS-3MIN.M  
 Catalog No : HY-10181 Batch#03040  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

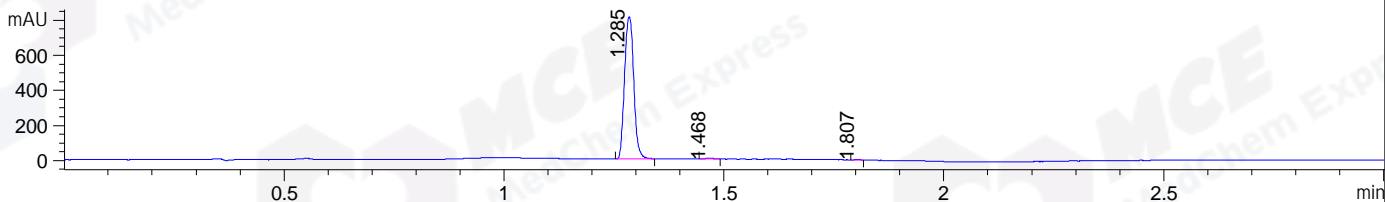


DAD1 C, Sig=254,4 Ref=off

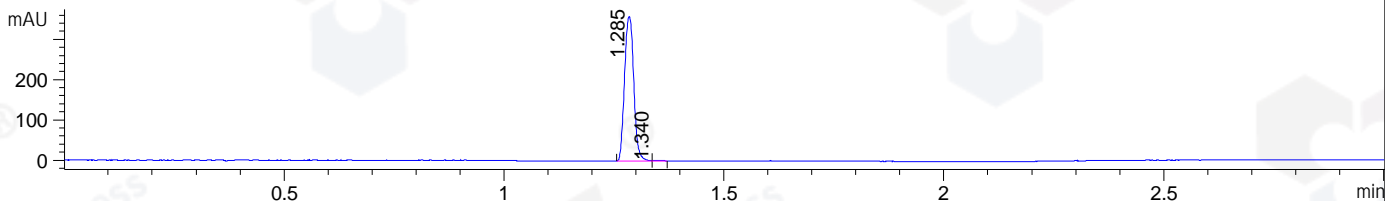

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

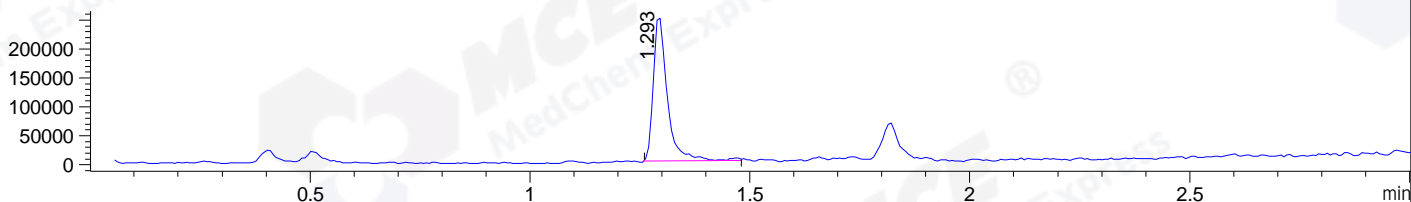

Ion 488, MSD1 488, Target Mass 487 +H Positive, EIC=487.7:488.7

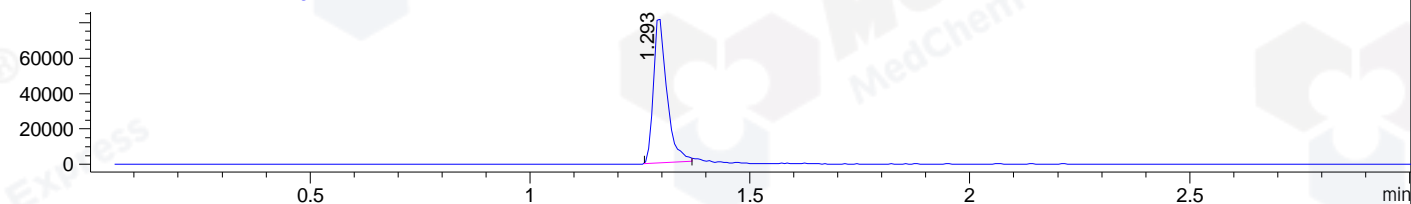

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.02	1178.71	811.82	99.48	488
1.47	0.03	4.74	3.02	0.40	ND
1.81	0.01	1.43	1.97	0.12	175

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.02	521.38	359.09	99.85	488
1.34	0.02	0.80	0.74	0.15	488

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.29	0.03	557337.94	252320.52	100.00	488

Ret. Time: 1.29

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

