



File ..ATA\2020\20200306\861 1\CPK2020-306-13039.D Tgt Mass (CHM):
 Injection Date : 6 Mar 20 6:07 pm +0800 Seq. Line : 101
 Sample Name : CPK2020-306-13039 Location : P1-B-01
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200306\861 1\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200306\861 1\1-POS-3MIN.M
 Catalog No : HY-10181A Batch# 13039
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

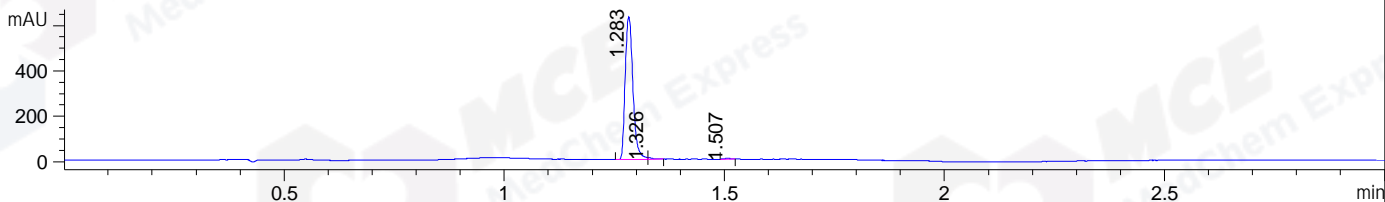


DAD1 C, Sig=254,4 Ref=off

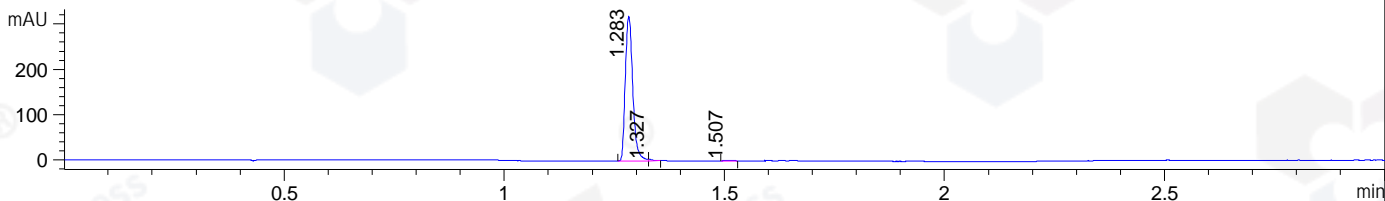

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

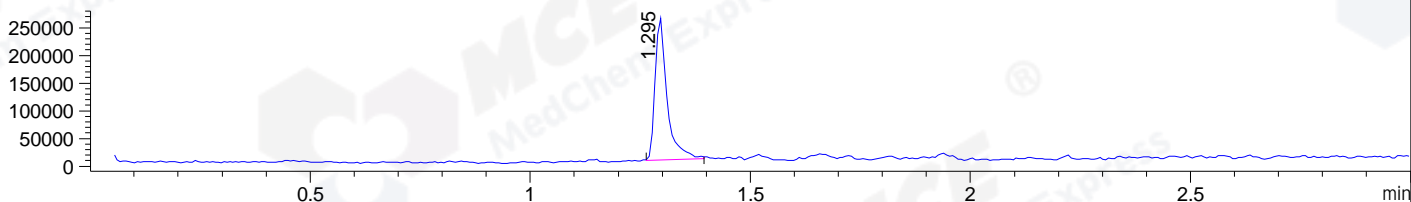

Ion 524, MSD1 524, Target Mass 523 +H Positive, EIC=523.7:524.7

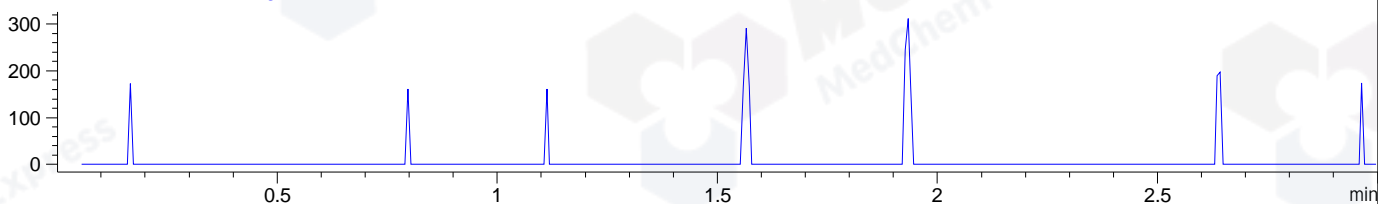

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.02	767.70	630.23	98.86	488
1.33	0.01	5.41	7.57	0.70	488
1.51	0.02	3.44	3.68	0.44	425

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.02	376.36	319.34	99.15	488
1.33	0.01	1.98	3.16	0.52	488
1.51	0.02	1.25	1.18	0.33	425

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.29	0.03	485832.31	258231.83	100.00	488

Ret. Time: 1.29

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

