


=====  
Acq. Operator : Li Shan(LCMS-02) Seq. Line : 50  
Acq. Instrument : HY-LCMS-02 Location : P1-E-04  
Injection Date : 4/1/2015 3:31:04 PM Inj : 1  
Inj Volume : 3.000 µl  
Acq. Method : D:\AGLIENT 1260\DATA\20150401\20150401 2015-04-01 09-07-02\100-1000MS+3MIN-1.5\_(0.02%FA).M  
Last changed : 4/1/2015 9:07:02 AM by Li Shan(LCMS-02)  
Analysis Method : D:\AGLIENT 1260\DATA\20150331\20150331 2015-03-31 09-21-27\100-1000MS+3MIN-1.5\_(0.02%FA).M (Sequence Method)  
Last changed : 4/1/2015 3:45:59 PM by Li Shan(LCMS-02)  
(modified after loading)  
Method Info : Postive,MS:100-1000,Column ID:A-RP-132,40°C  
Catalog No : HY-10200 Batch#08106  
A-RP-132

Additional Info : Peak(s) manually integrated

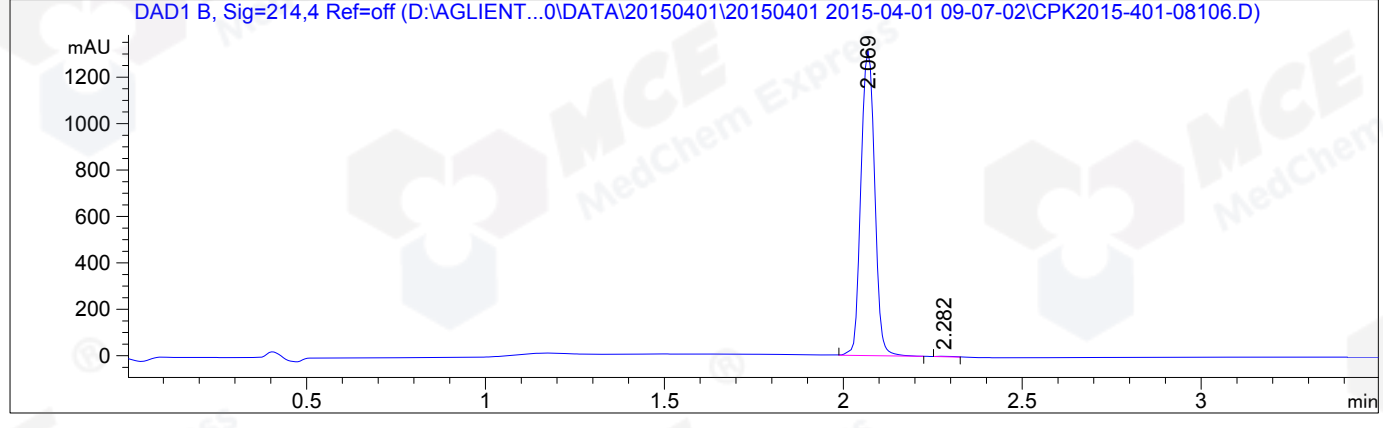

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 B, Sig=214,4 Ref=off

| Peak # | RetTime [min] | Type | Width [min] | Area [mAU*s] | Height [mAU] | Area %  |
|--------|---------------|------|-------------|--------------|--------------|---------|
| 1      | 2.069         | MM   | 0.0444      | 3514.36597   | 1319.17017   | 99.7882 |
| 2      | 2.282         | MM   | 0.0440      | 7.45989      | 2.82763      | 0.2118  |


Totals : 3521.82586 1321.99780

=====  
\*\*\* End of Report \*\*\*  
=====

=====


|                 |  |            |            |
|-----------------|--|------------|------------|
| Acq. Operator   | : Li Shan (LCMS-02)  | Seq. Line  | : 50       |
| Acq. Instrument | : HY-LCMS-02   | Location   | : P1-E-04  |
| Injection Date  | : 4/1/2015 3:31:04 PM  | Inj        | : 1        |
|                 |  | Inj Volume | : 3.000 µl |
| Acq. Method     | : D:\AGLIENT 1260\DATA\20150401\20150401 2015-04-01 09-07-02\100-1000MS+3MIN-1.5_(0.02%FA).M                   |            |            |
| Last changed    | : 4/17/2015 9:07:02 AM by Li Shan (LCMS-02)  |            |            |
| Analysis Method | : D:\AGLIENT 1260\DATA\20150331\20150331 2015-03-31 09-21-27\100-1000MS+3MIN-1.5_(0.02%FA).M (Sequence Method) |            |            |
| Last changed    | : 4/17/2015 3:47:17 PM by Li Shan (LCMS-02)<br>(modified after loading)  |            |            |
| Method Info     | : Postive,MS:100-1000,Column ID:A-RP-132,40°C  |            |            |
| Catalog No      | : HY-10200 Batch#08106<br>A-RP-132   |            |            |

Additional Info : Peak(s) manually integrated

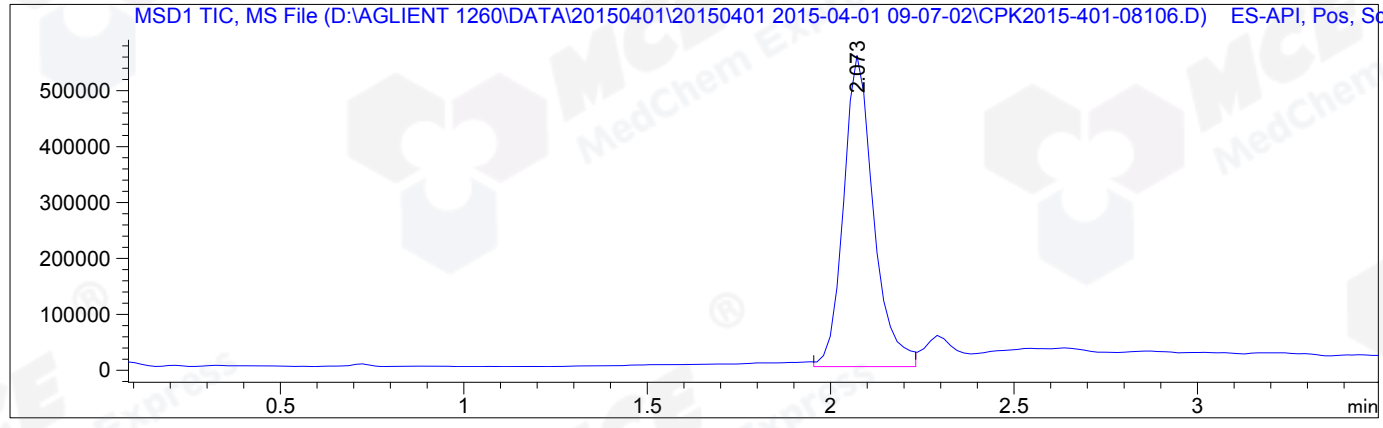

MS Signal: MSD1 TIC, MS File, ES-API, Pos, Scan, Frag: 50  
Spectra averaged over upper half of peaks.  
Noise Cutoff: 1000 counts.  
Reportable Ion Abundance: > 10%.

| Retention Time (MS) | MS Area | Mol. Weight or Ion   |
|---------------------|---------|----------------------|
| 2.073               | 3151808 | 462.90 I<br>461.90 I |

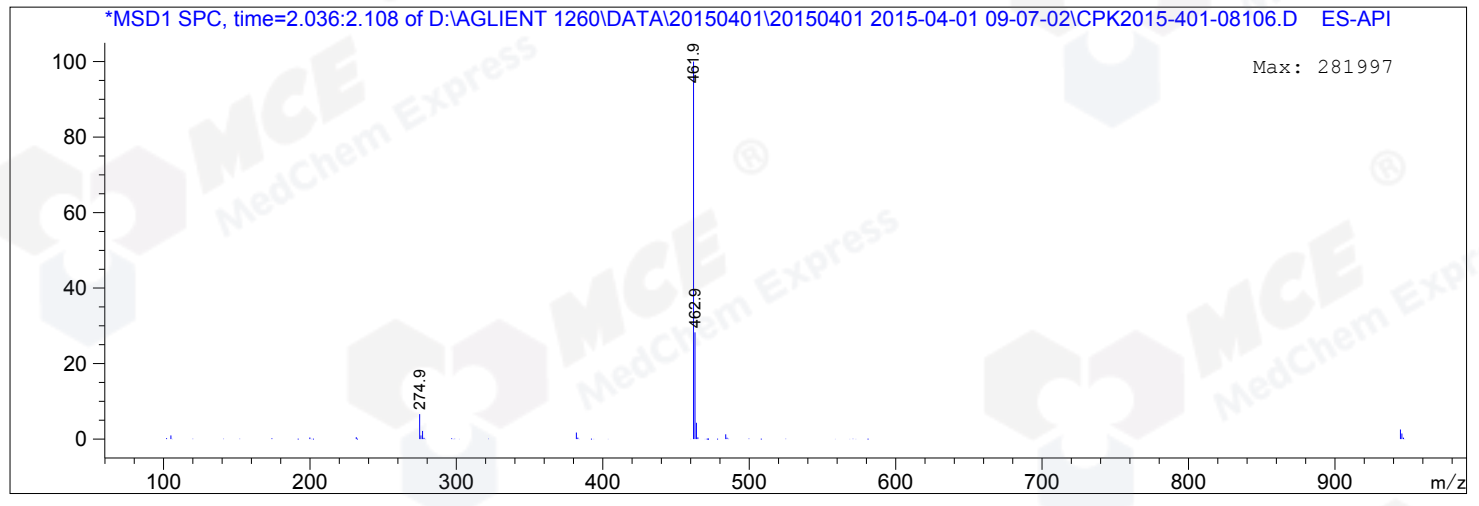

\*\*\* End of Report \*\*\*