

File ..DATA\2020\20200328\898\CPK2020-324-26078-.D Tgt Mass (CHM):

Injection Date : 28 Mar 20 7:52 pm +0800 Seq. Line : 125

Sample Name : CPK2020-324-26078 Location : P1-E-04

Acq. Operator : LQ\_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.4 ul

Acq. Method : D:\Chem32\1\data\2020\20200328\898\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200328\898\1-POS-3MIN.M

Catalog No : HY-103022 Batch#26078

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

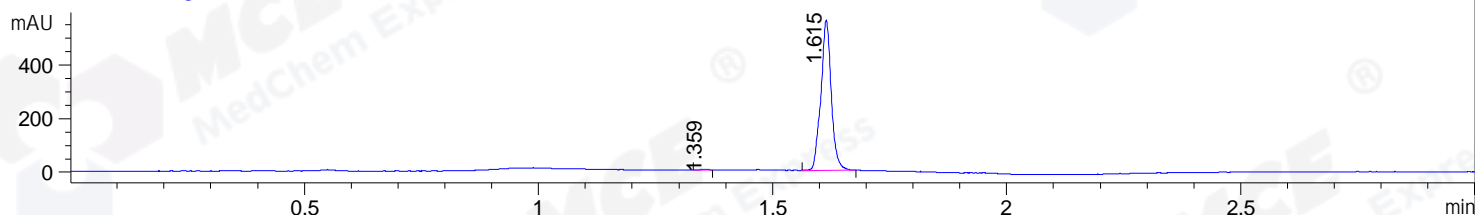


DAD1 C, Sig=254,4 Ref=off

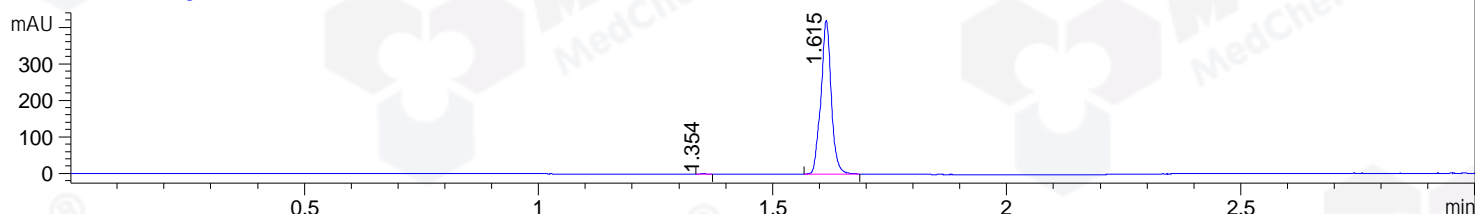

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

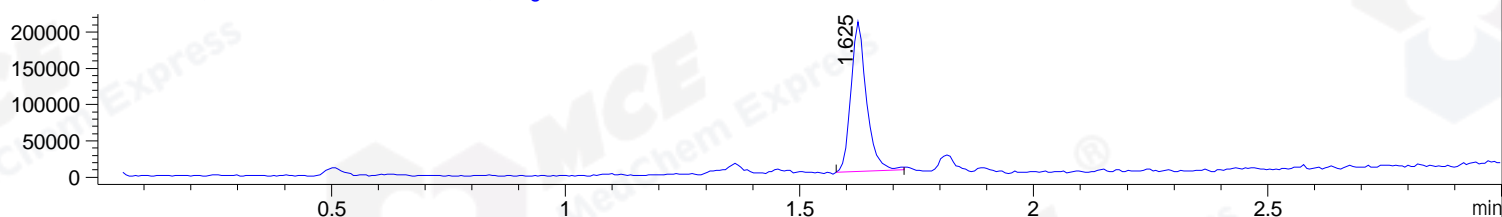

Ion 356, MSD1 356, Target Mass 355 +H Positive, EIC=355.7:356.7

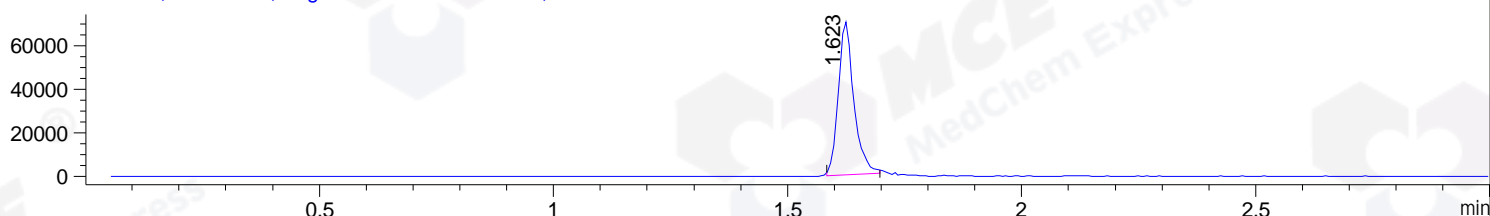

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.02	2.68	1.93	0.31	ND
1.61	0.03	865.38	561.46	99.69	356

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.02	1.20	1.24	0.19	ND
1.61	0.03	646.41	421.08	99.81	356

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.62	0.03	478540.88	206940.03	100.00	356

Ret. Time: 1.62

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

