



File ..DATA\2021\20210123\1244\CPK2021-122-18916.D Tgt Mass (CHM):
 Injection Date : 23 Jan 21 10:31 am +0800 Seq. Line : 19
 Sample Name : CPK2021-122-18916 Location : P1-D-03
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210123\1244\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210123\1244\1-POS-3MIN.M
 CAS NO. : 1032350-13-2
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

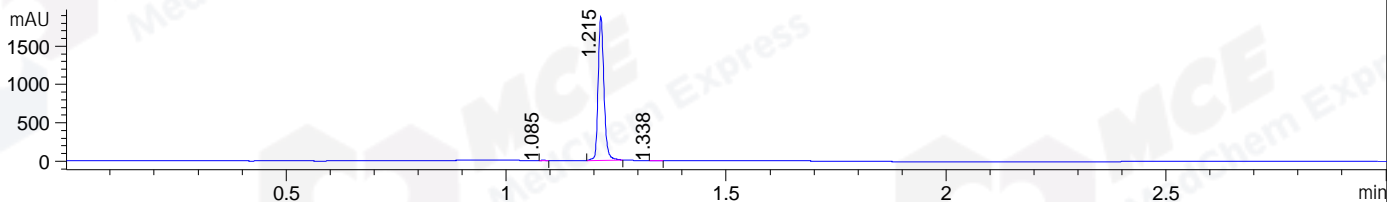


DAD1 C, Sig=254,4 Ref=off

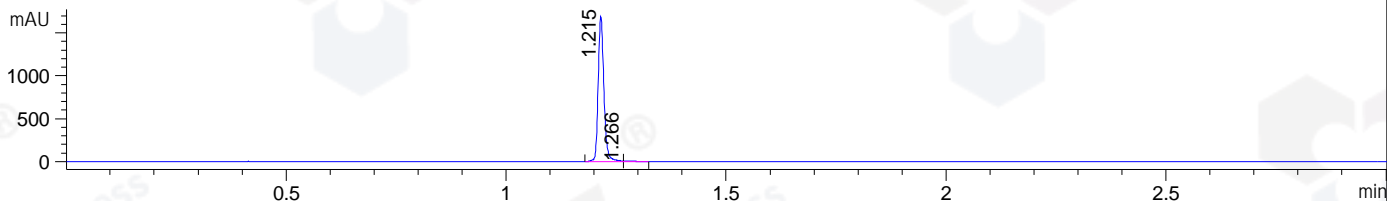

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

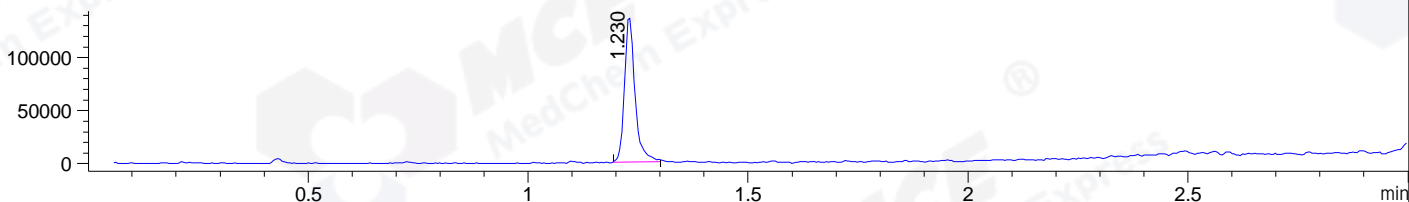

Ion 408, MSD1 408, Target Mass 407 +H Positive, EIC=407.7:408.7

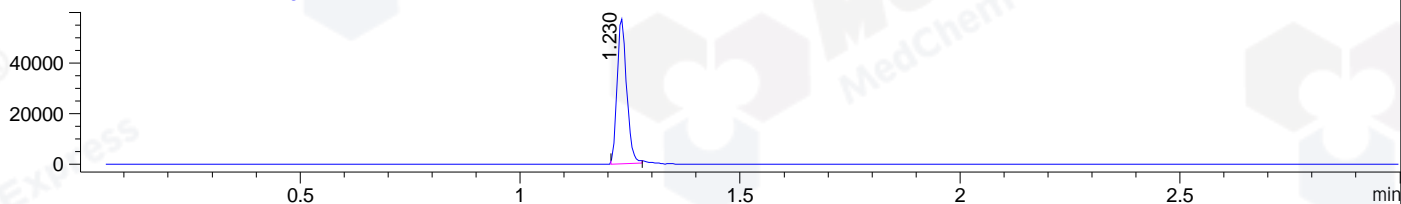

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.01	1.80	2.48	0.10	ND
1.22	0.02	1715.26	1876.36	99.76	408
1.34	0.02	2.40	2.14	0.14	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.02	1529.07	1695.63	99.47	408
1.27	0.02	8.21	6.67	0.53	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.02	228926.77	138273.73	100.00	408

Ret. Time: 1.23

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

