

File ..\DATA\2020\20200722\1049\BIZ2020-721-SCH2.D Tgt Mass (CHM):

Injection Date : 22 Jul 20 11:18 am +0800 Seq. Line : 29

Sample Name : BIZ2020-721-SCH2 Location : PL-B-02

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2020\20200722\1049\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200722\1049\1-POS-3MIN.M

Catalog No : HY-103647

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-607

Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

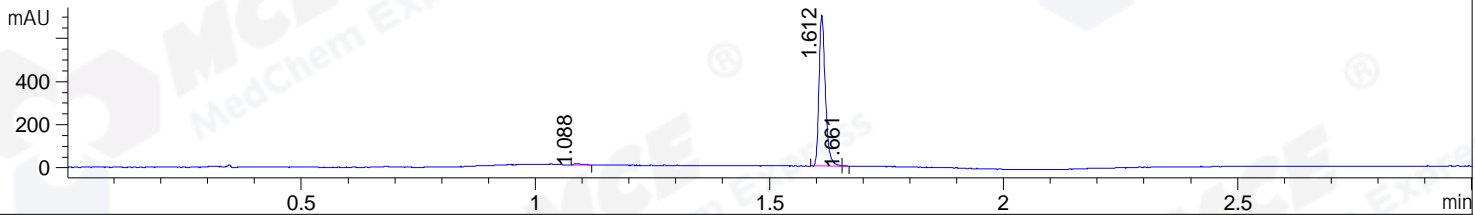


DAD1 C, Sig=254,4 Ref=off

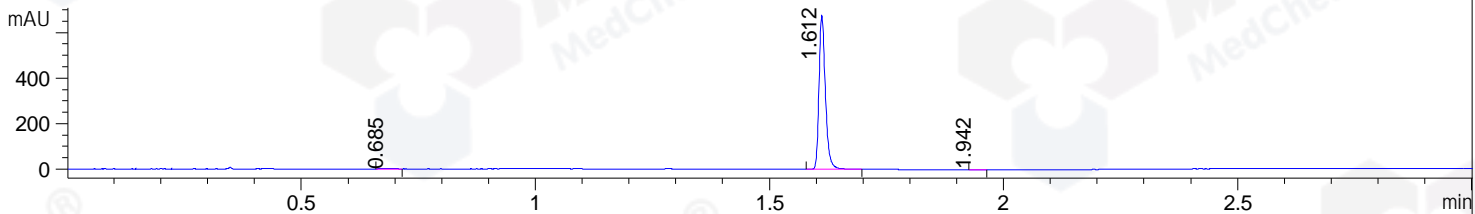

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

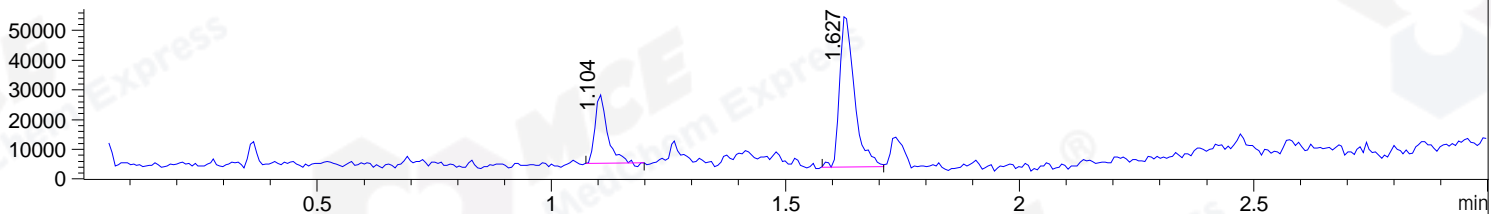

Ion 426, MSD1 426, Target Mass 425 +H Positive, EIC=425.7:426.7

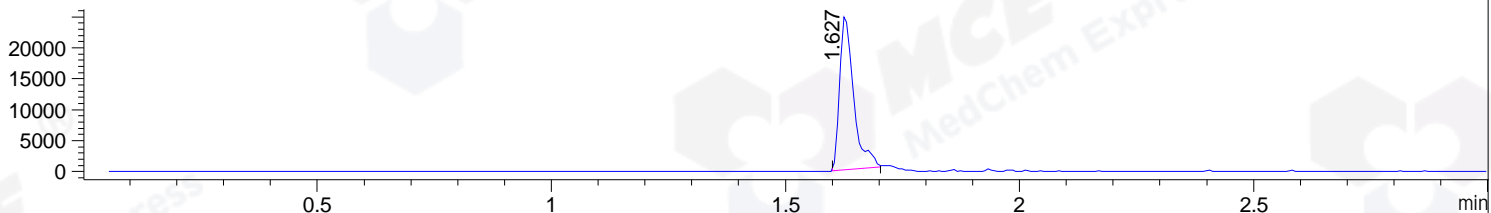

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.02	6.78	6.32	1.01	209
1.61	0.02	660.74	701.44	98.78	426
1.66	0.01	1.38	2.40	0.21	426

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.69	0.03	2.43	1.41	0.37	252
1.61	0.02	644.59	678.11	99.46	426
1.94	0.02	1.08	1.10	0.17	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.03	41881.45	23042.98	27.08	209
1.63	0.04	112802.50	52235.56	72.92	426

Ret. Time: 1.10

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.63

ES-API Positive

