



File ..019\20190702\20190702 1\CPK2019-701-15641.D Tgt Mass (CHM):  
 Injection Date : 2 Jul 19 2:59 pm +0800 Seq. Line : 50  
 Sample Name : CPK2019-701-15641 Location : P2-A-05  
 Acq. Operator : SYSTEM Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 3 ul  
 Acq. Method : D:\LCMS03\Data\20190702\20190702 1\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2019\20190702\20190702 1\1-POS-3MIN.M  
 Catalog No : HY-10421 Batch#15641  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-446  
 Oven Temperature : 45C


DAD1 B, Sig=254,4 Ref=off

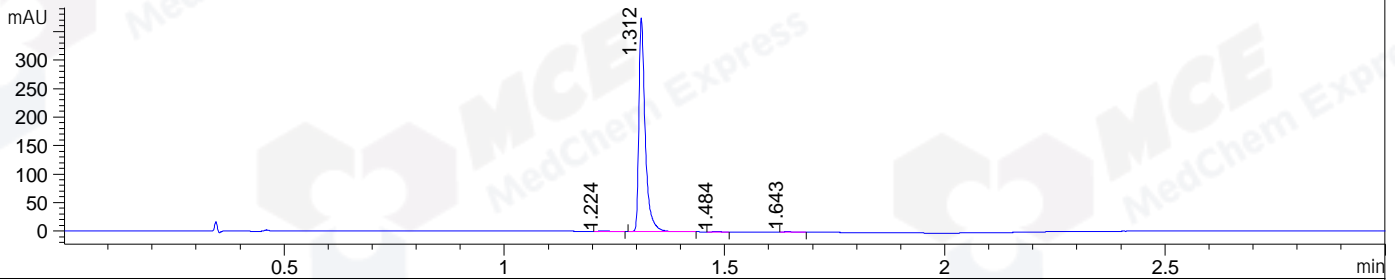

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

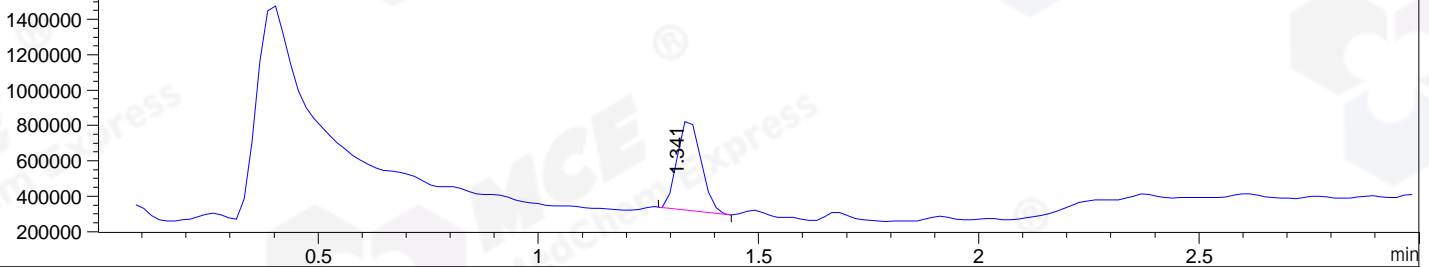

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

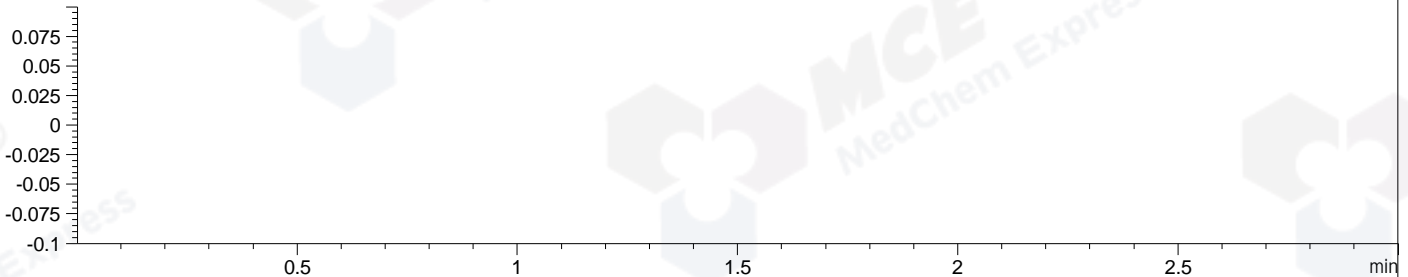

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.02	0.90	0.70	0.24	145
1.31	0.02	372.65	374.18	99.36	145
1.48	0.02	0.38	0.32	0.10	145
1.64	0.02	1.11	1.08	0.30	145

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.34	0.06	1909064.00	519871.53	100.00	145

Ret. Time: 1.34

<<<< POSITIVE SPECTRA >>>>

