


46 CPK2019-N05-03096 sd**Catalog No: HY-10422 Batch#03096 A-RP-243 JLW**

Sample Name:	CPK2019-N05-03096	Injection Volume:	2.0
Vial Number:	GE2	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	236
Control Program:	10-80A,236NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-11-6 2:12	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

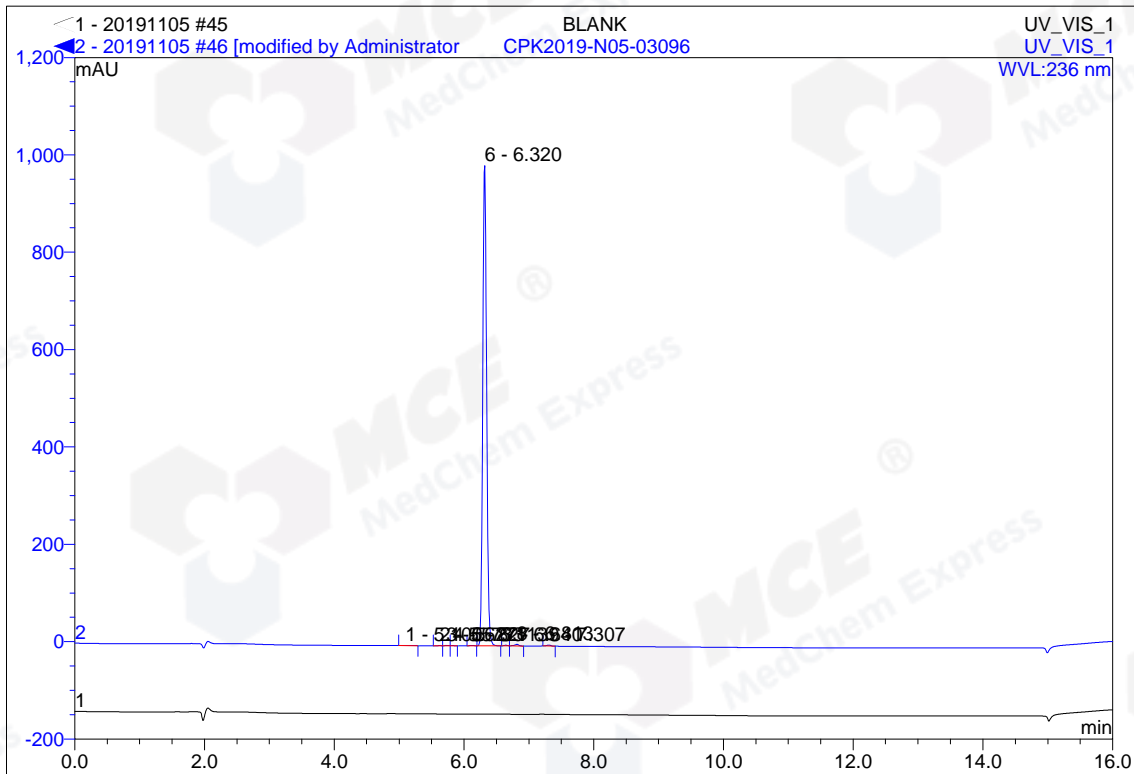

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	5.10	n.a.	0.391	0.033	0.05	n.a.	BMB
2	5.63	n.a.	0.245	0.016	0.02	n.a.	BM *
3	5.73	n.a.	0.420	0.034	0.05	n.a.	M *
4	5.83	n.a.	0.321	0.021	0.03	n.a.	MB*
5	6.11	n.a.	0.373	0.030	0.04	n.a.	BMB*
6	6.32	n.a.	986.519	67.778	99.19	n.a.	BMB
7	6.64	n.a.	1.025	0.057	0.08	n.a.	BMB
8	6.81	n.a.	3.034	0.221	0.32	n.a.	bMB
9	7.31	n.a.	1.875	0.142	0.21	n.a.	BMB*
Total:			994.206	68.332	100.00	0.000	