


Mass Spectrum

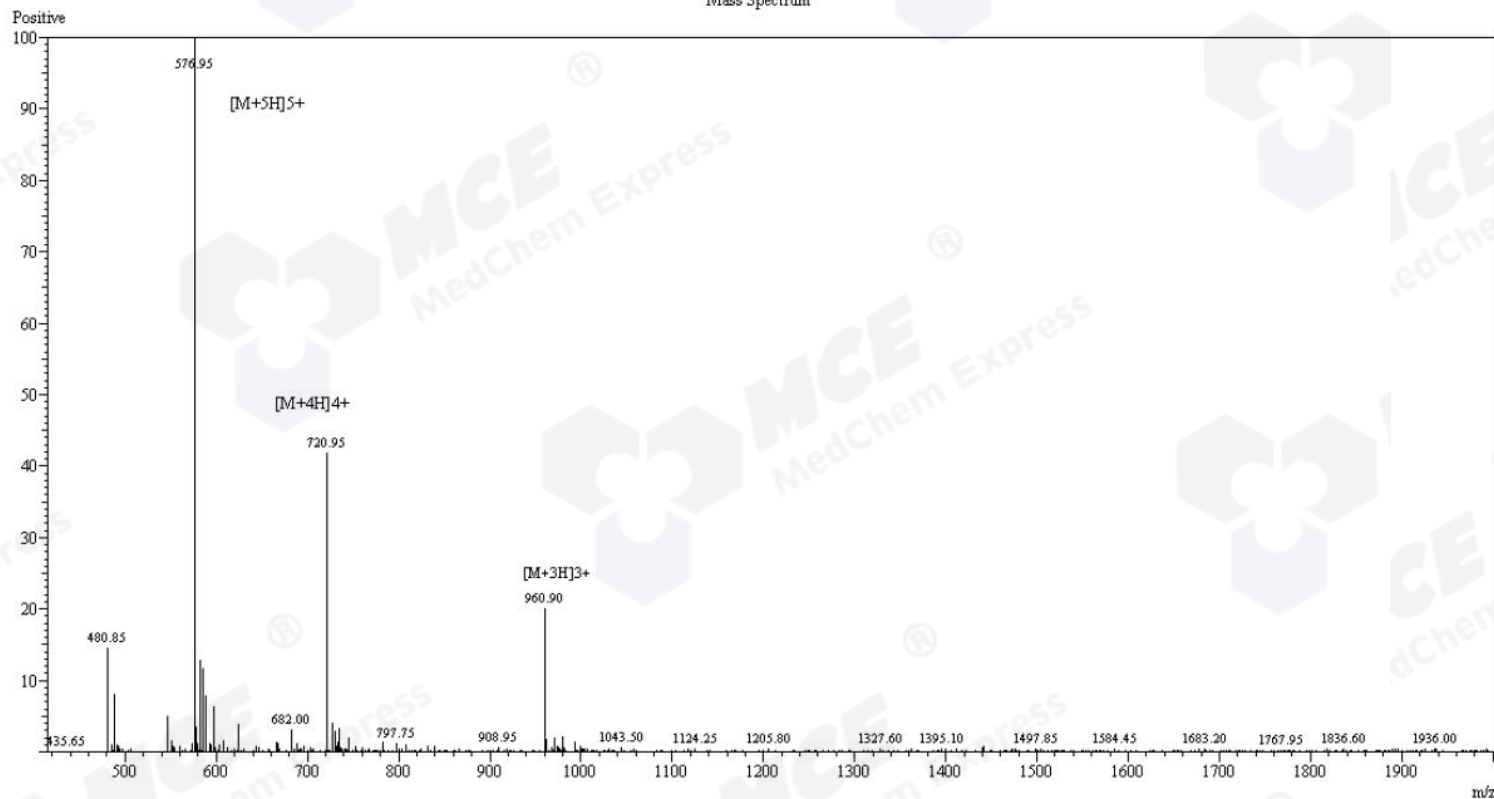

Sample Information

Date and Time : 2018-7-31 13:52:02
 User : CHAO
 Sample : 949100-39-4 CL-23
 Inj. Volume : 1
 MW : 2880.29
 Catalog No : HY-106262 Batch#32133

Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 DL: -20.0V
 DL Temp: 250°C
 Block Temp: 200°C
 Probe bias: -3.5kv
 Detector: 1.0kv
 T. Flow: 0.2ml/min
 B. conc: 50%H₂O/50%ACN