



File ..DATA\2020\20200927\1118\CPK2020-927-08221.D Tgt Mass (CHM):  
Injection Date : 27 Sep 20 12:23 pm +0800 Seq. Line : 34  
Sample Name : CPK2020-927-08221 Location : P1-A-07  
Acq. Operator : zyj\_1547 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20200927\1118\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200927\1118\1-POS-3MIN.M  
CAS NO. : 501951-42-4  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

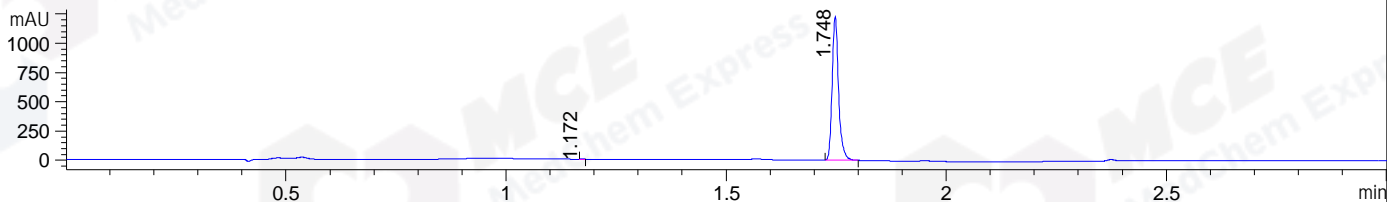


DAD1 C, Sig=254,4 Ref=off

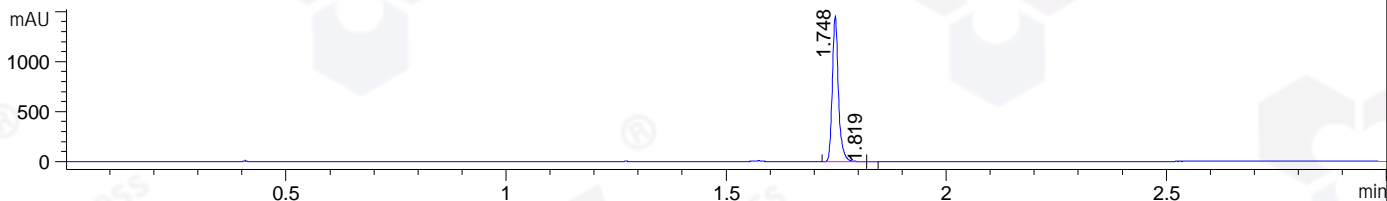

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

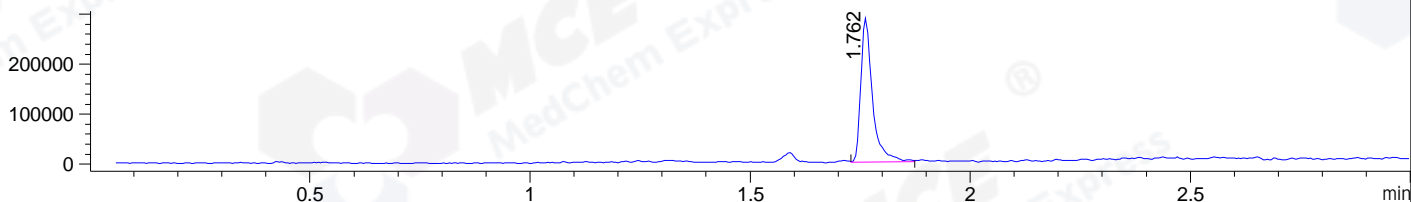

Ion 429, MSD1 429, Target Mass 428 +H Positive, EIC=428.7:429.7

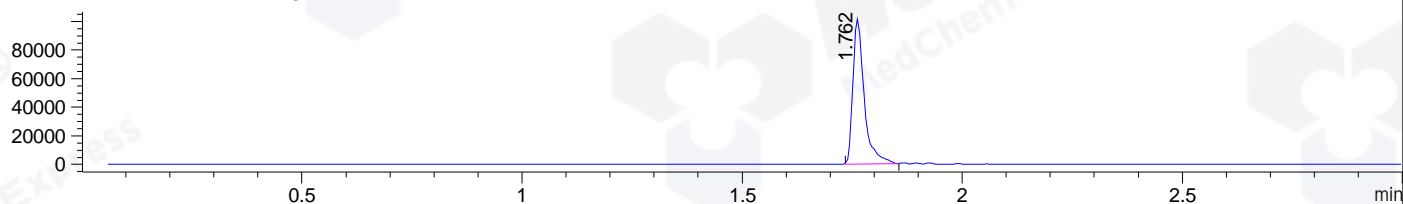

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.01	0.29	0.52	0.02	ND
1.75	0.02	1235.51	1229.13	99.98	431

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.75	0.02	1404.85	1457.99	99.96	431
1.82	0.01	0.61	0.68	0.04	429

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.76	0.03	533463.63	288327.09	100.00	431

Ret. Time: 1.76

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

