



File ..\DATA\2020\20200806\1064\BIZ2020-805-WMX4.D Tgt Mass (CHM):  
 Injection Date : 6 Aug 20 3:28 pm +0800 Seq. Line : 69  
 Sample Name : BIZ2020-805-WMX4 Location : P1-C-01  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200806\1064\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200806\1064\1-POS-3MIN.M  
 Catalog No : HY-106994A  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314  
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

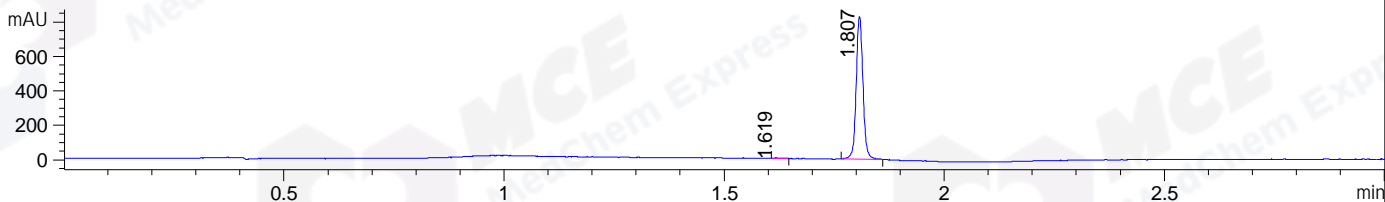


DAD1 C, Sig=254,4 Ref=off

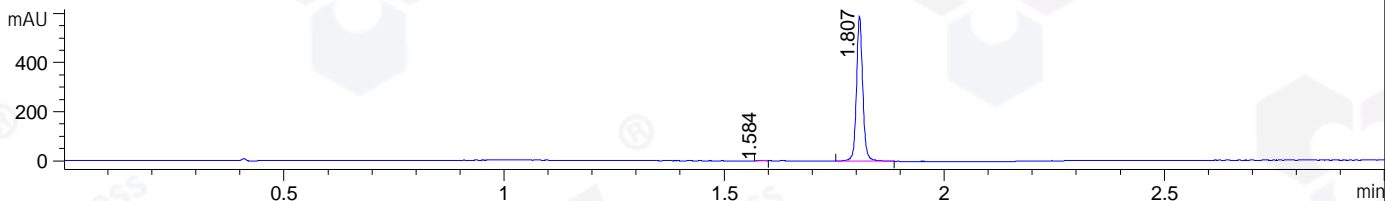

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

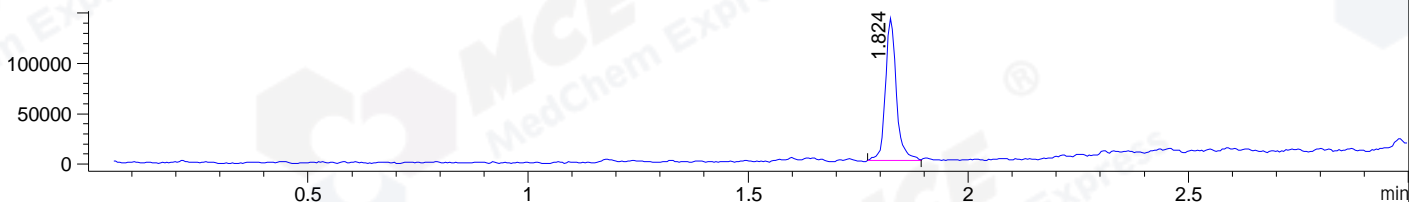

Ion 492, MSD1 492, Target Mass 491 +H Positive, EIC=491.7:492.7

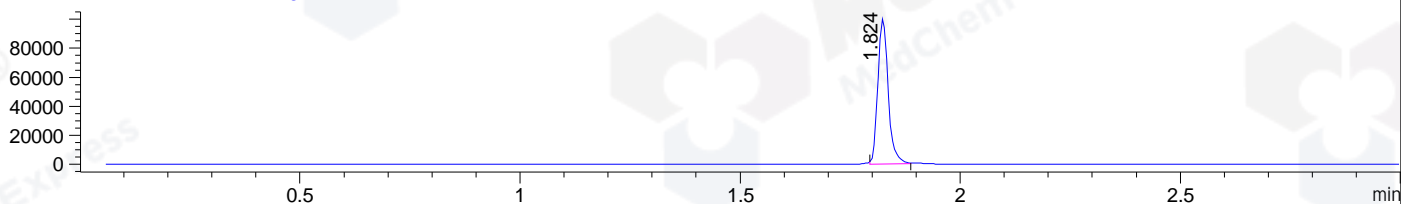

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.62	0.03	4.17	2.78	0.47	ND
1.81	0.02	886.18	827.27	99.53	492

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.58	0.01	2.17	2.48	0.37	ND
1.81	0.02	587.05	589.98	99.63	492

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.82	0.03	241749.77	141620.77	100.00	492

Ret. Time: 1.82

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

