
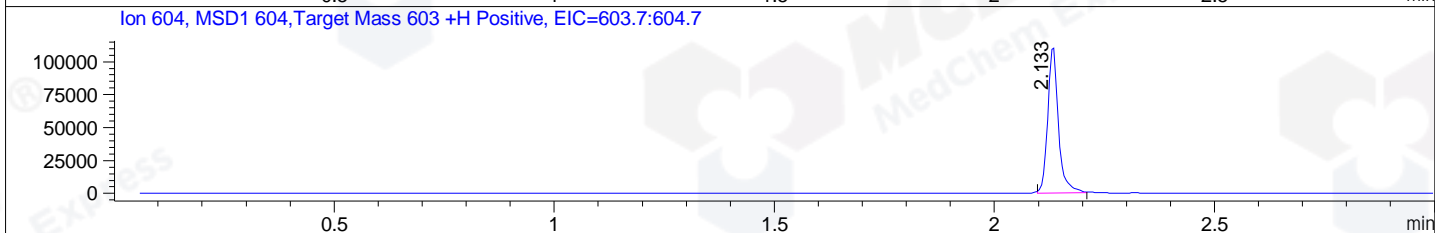
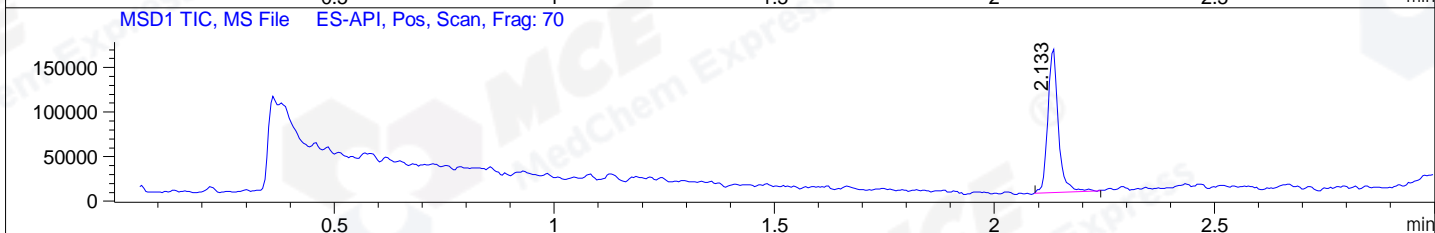
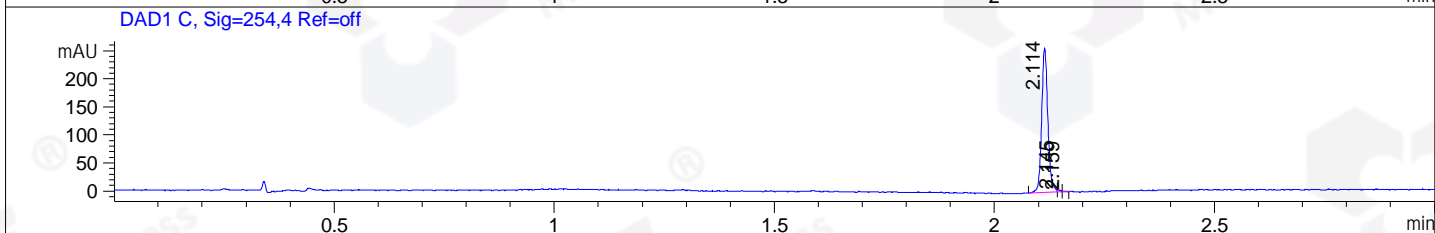


File ..DATA\2020\20200820\1077\CPK2020-818-28677.D Tgt Mass (CHM):
 Injection Date : 20 Aug 20 1:00 pm +0800 Seq. Line : 44
 Sample Name : CPK2020-818-28677 Location : P1-E-01
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 2 ul
 Acq. Method : D:\Chem32\1\data\2020\20200820\1077\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200820\1077\1-POS-3MIN.M
 Catalog No : HY-107418
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45C

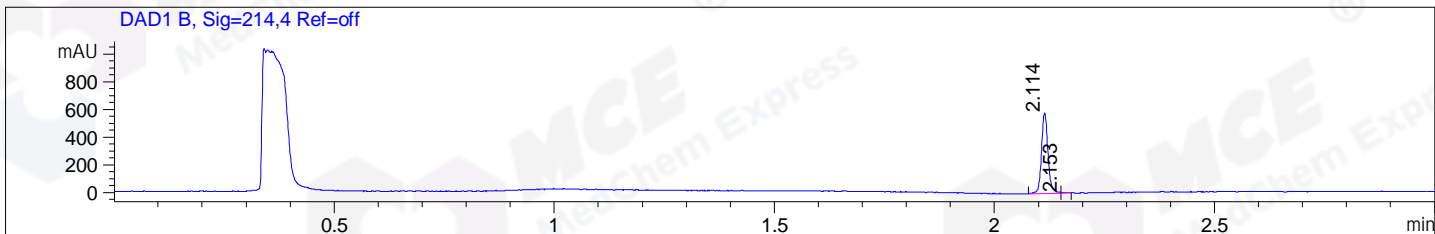

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.11	0.02	594.93	581.19	99.35	604
2.15	0.01	3.88	4.52	0.65	604

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.11	0.02	252.39	257.69	98.98	604
2.14	0.01	1.77	3.59	0.69	604
2.16	0.01	0.84	1.58	0.33	604

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.13	0.02	268212.34	163295.34	100.00	604

Ret. Time: 2.13

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

