



File ..DATA\2020\20200924\1116\CPK2020-924-28738.D Tgt Mass (CHM):  
 Injection Date : 24 Sep 20 1:10 pm +0800 Seq. Line : 51  
 Sample Name : CPK2020-924-28738 Location : P1-B-04  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200924\1116\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200924\1116\1-POS-3MIN.M  
 Catalog No : HY-107500  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

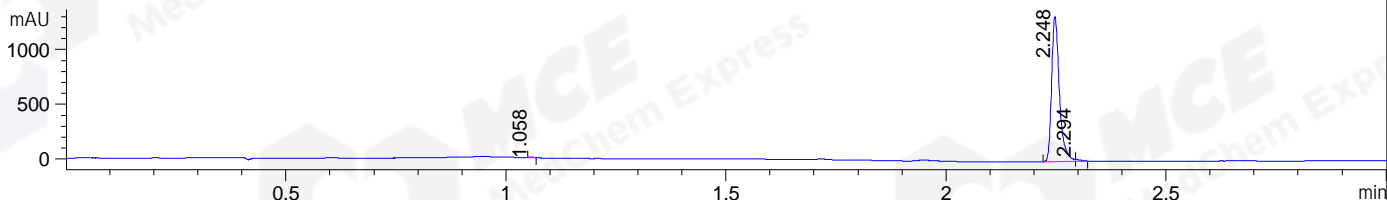


DAD1 C, Sig=254,4 Ref=off

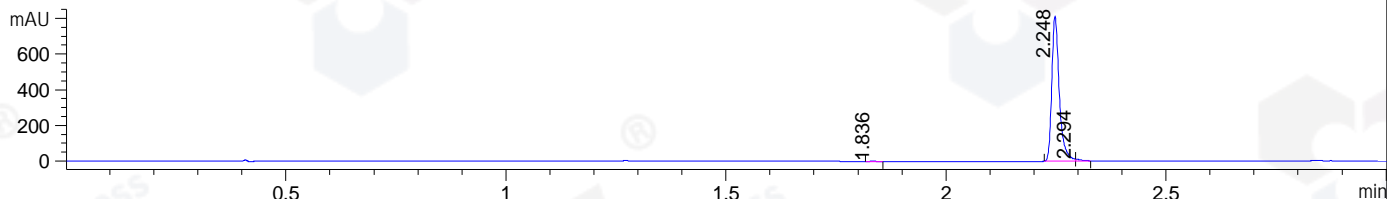

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

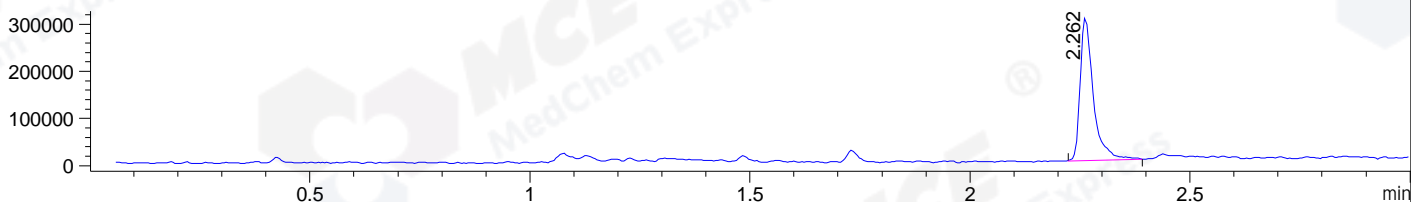

Ion 437, MSD1 437, Target Mass 436 +H Positive, EIC=436.7:437.7

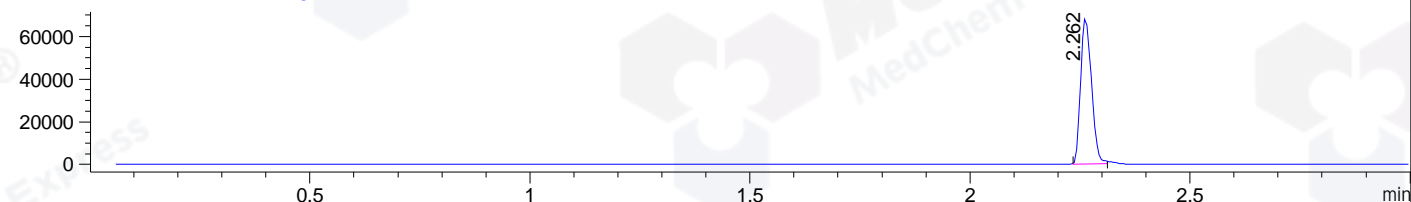

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.01	3.67	5.50	0.22	223
2.25	0.02	1627.45	1325.14	99.03	419
2.29	0.01	12.22	16.34	0.74	419

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.84	0.02	1.14	0.89	0.12	ND
2.25	0.02	963.63	813.77	99.02	419
2.29	0.01	8.42	10.38	0.87	419

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.26	0.03	630095.94	302589.97	100.00	419

Ret. Time: 2.26

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

