



File ..DATA\2021\20210106\1227\CPK2021-106-30279.D Tgt Mass (CHM):
Injection Date : 6 Jan 21 4:54 pm +0800 Seq. Line : 89
Sample Name : CPK2021-106-30279 Location : P1-E-03
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2021\20210106\1227\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2021\20210106\1227\1-POS-3MIN.M
CAS NO. : 1039758-22-9
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

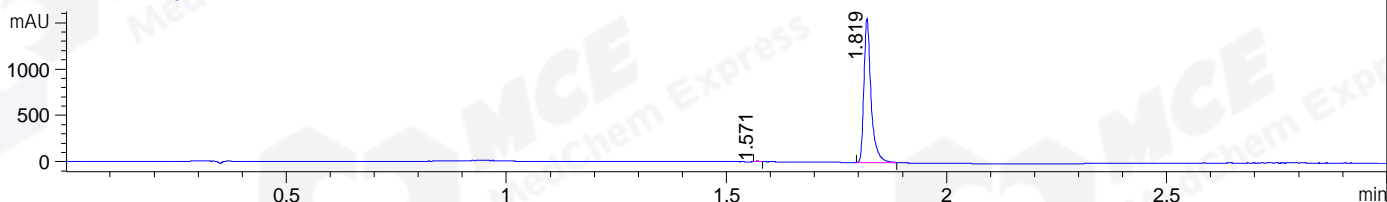


DAD1 C, Sig=254,4 Ref=off

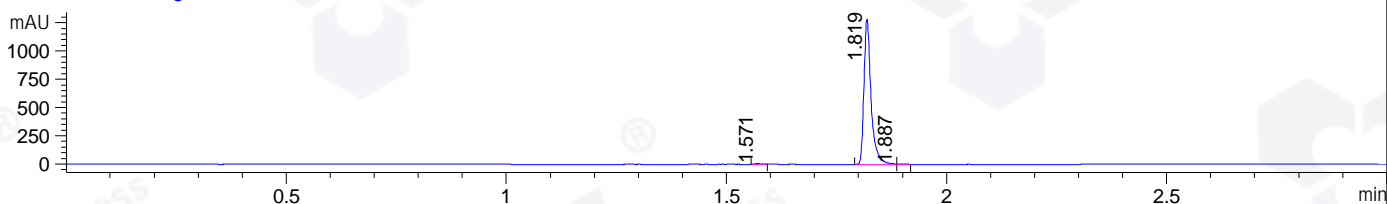

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

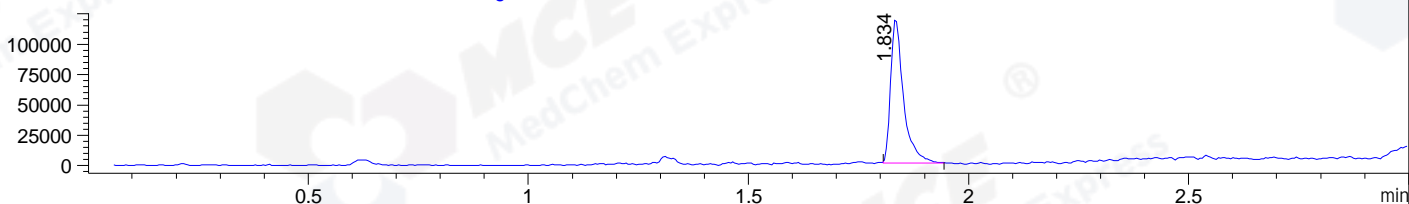

Ion 566, MSD1 566, Target Mass 565 +H Positive, EIC=565.7:566.7

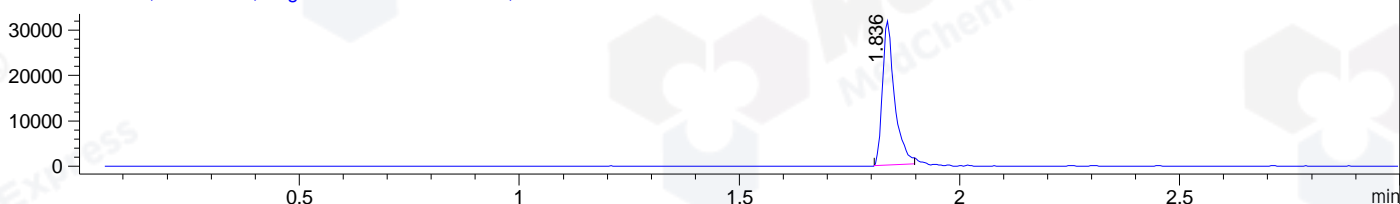

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.57	0.01	5.13	6.68	0.29	ND
1.82	0.02	1745.89	1553.73	99.71	284

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.57	0.02	5.70	6.08	0.39	ND
1.82	0.02	1447.42	1283.34	99.28	284
1.89	0.02	4.85	4.65	0.33	284

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.83	0.03	242189.70	119554.63	100.00	284

Ret. Time: 1.83

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

