


7 CPK2019-N20-08404**Catalog No : HY-10809A Batch# 08404 A-RP-234 JLW**

Sample Name:	CPK2019-N20-08404	Injection Volume:	5.0
Vial Number:	BE6	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	210
Control Program:	HM-261_10B-H01P01(RP-HPLC)	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-11-22 14:14	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

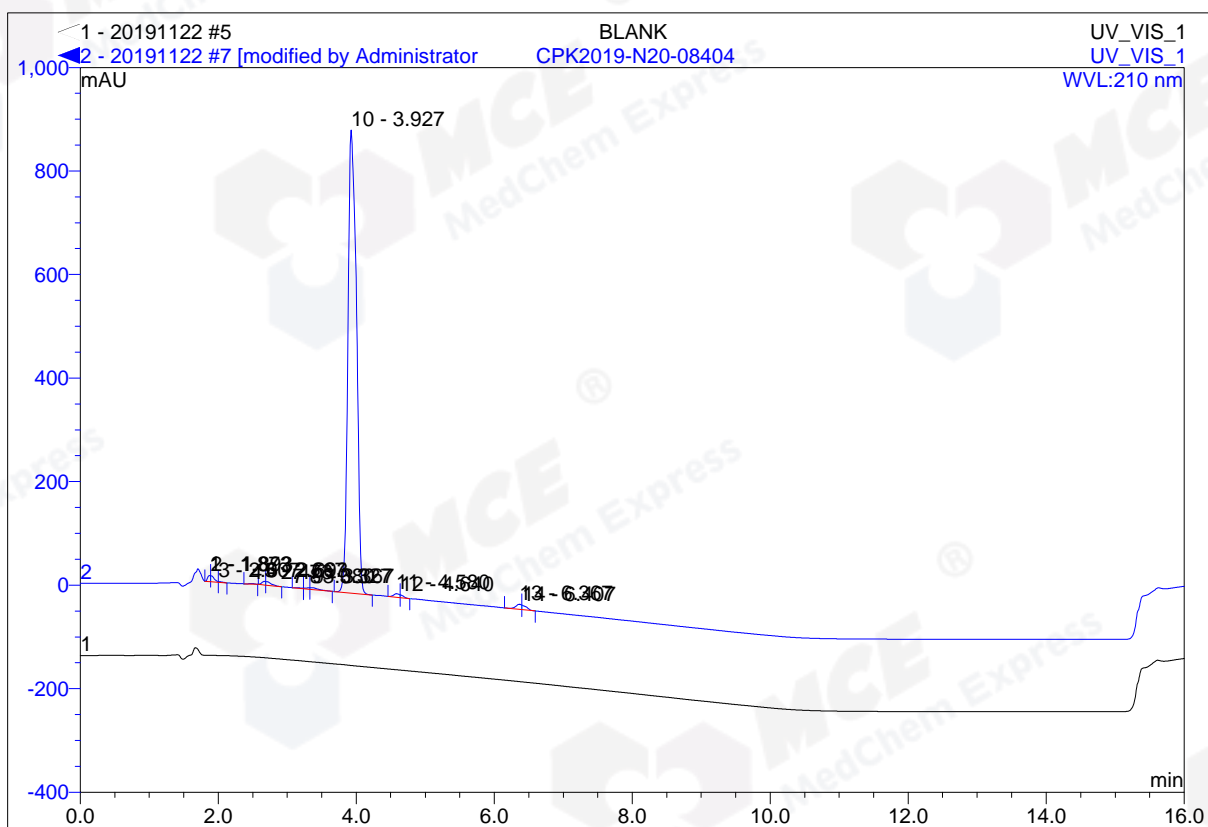

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	1.87	n.a.	11.652	0.522	0.39	n.a.	BM *
2	1.89	n.a.	11.230	0.712	0.54	n.a.	M *
3	2.01	n.a.	1.372	0.100	0.08	n.a.	MB*
4	2.47	n.a.	0.857	0.087	0.07	n.a.	BMB*
5	2.67	n.a.	6.691	0.409	0.31	n.a.	BM *
6	2.69	n.a.	6.651	0.619	0.47	n.a.	MB*
7	3.08	n.a.	0.025	0.094	0.07	n.a.	BM *
8	3.33	n.a.	2.704	0.176	0.13	n.a.	M *
9	3.37	n.a.	3.608	0.453	0.34	n.a.	MB*
10	3.93	n.a.	894.873	127.330	95.68	n.a.	BMB*
11	4.58	n.a.	6.887	0.644	0.48	n.a.	BM *
12	4.64	n.a.	5.195	0.315	0.24	n.a.	MB*
13	6.37	n.a.	9.944	0.923	0.69	n.a.	BM
14	6.41	n.a.	8.234	0.692	0.52	n.a.	MB
Total:			969.924	133.077	100.00	0.000	