
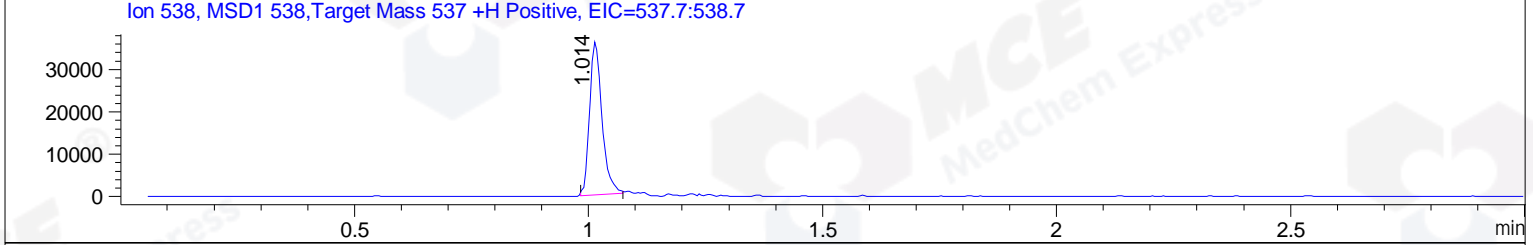




File ..DATA\2020\20200904\1098\BIZ2020-903-SCH12.D Tgt Mass (CHM):  
 Injection Date : 4 Sep 20 2:32 pm +0800 Seq. Line : 72  
 Sample Name : BIZ2020-903-SCH12 Location : P1-A-08  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200904\1098\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200904\1098\1-POS-3MIN.M  
 Catalog No : HY-108631  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45C



Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.00	0.02	1977.54	1813.77	99.72	538
1.15	0.02	5.55	4.16	0.28	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.00	0.02	950.47	950.09	99.65	538
1.16	0.02	3.38	2.29	0.35	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.01	0.03	136323.17	69726.18	100.00	538

Ret. Time: 1.01

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

