



File ..\DATA\2020\20201020\1130\BIZ2020-O17-SCH7.D Tgt Mass (CHM):
Injection Date : 20 Oct 20 2:02 pm +0800 Seq. Line : 56
Sample Name : BIZ2020-O17-SCH7 Location : P1-B-01
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201020\1130\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201020\1130\1-POS-3MIN.M
CAS NO. : 1513857-77-6
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

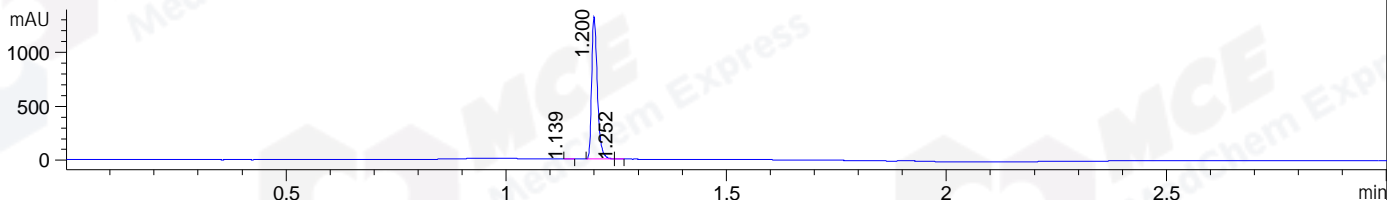


DAD1 C, Sig=254,4 Ref=off

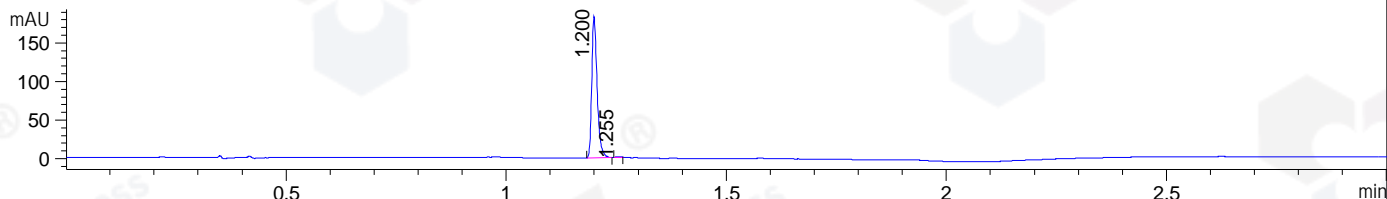

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

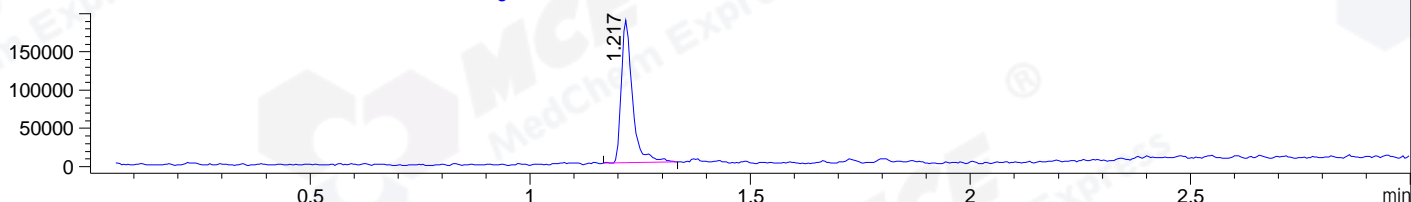

Ion 488, MSD1 488, Target Mass 487 +H Positive, EIC=487.7:488.7

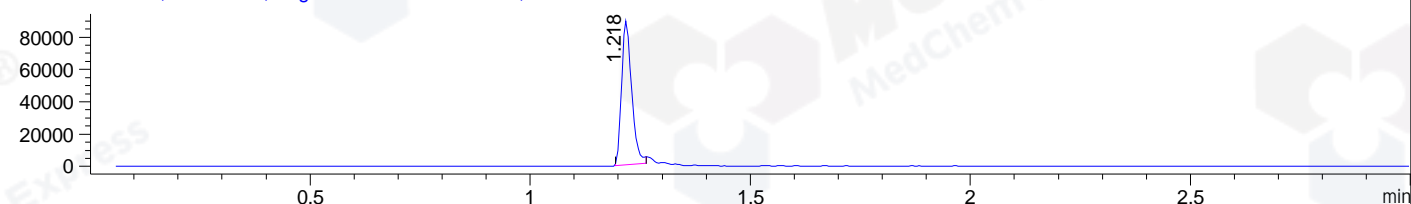

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.14	0.01	1.50	1.99	0.13	ND
1.20	0.01	1186.97	1318.87	99.73	488
1.25	0.01	1.72	2.13	0.14	488

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.01	154.67	183.66	99.54	488
1.25	0.01	0.72	1.08	0.46	488

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.03	327492.16	186628.02	100.00	488

Ret. Time: 1.22

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

