


=====  
Acq. Operator : Su Xiao Ying(LCMS-02) Seq. Line : 48  
Acq. Instrument : HY-LCMS-02 Location : P1-B-05  
Injection Date : 5/6/2016 2:08:37 PM Inj : 1  
Inj Volume : 3.000 µl  
Acq. Method : D:\AGLIENT 1260\DATA\20160506\20160506 2016-05-06 08-43-06\100-1000MS+3MIN-1.5\_(0.02%FA).M  
Last changed : 5/6/2016 8:43:06 AM by Su Xiao Ying(LCMS-02)  
Analysis Method : D:\AGLIENT 1260\DATA\20160506\20160506 2016-05-06 08-43-06\100-1000MS+3MIN-1.5\_(0.02%FA).M (Sequence Method)  
Last changed : 5/6/2016 2:14:30 PM by Su Xiao Ying(LCMS-02)  
(modified after loading)  
Method Info : HY-365\_5H01RS,M,A-RP-108, 210nm,23min  
Catalog No : HY-10943 Batch#20311  
A-RP-134

Additional Info : Peak(s) manually integrated

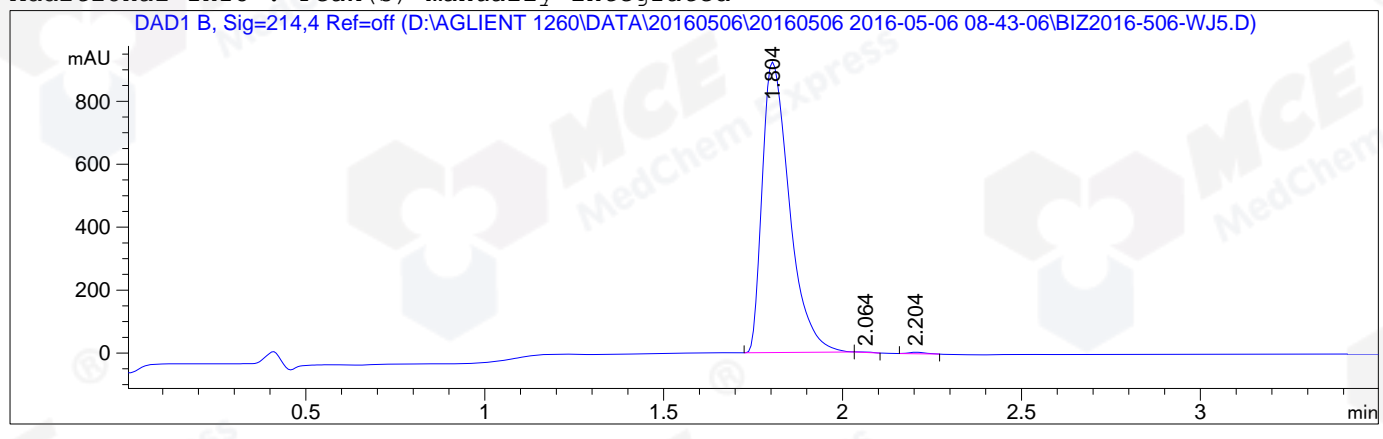

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 B, Sig=214,4 Ref=off


Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.804	MM	0.0879	4883.36230	925.47675	99.6368
2	2.064	MM	0.0370	3.47323	1.56649	0.0709
3	2.204	MM	0.0491	14.32536	4.86601	0.2923

Totals : 4901.16090 931.90925

=====  
\*\*\* End of Report \*\*\*  
=====


=====  
Acq. Operator : Su Xiao Ying(LCMS-02) Seq. Line : 48  
Acq. Instrument : HY-LCMS-02 Location : P1-B-05  
Injection Date : 5/6/2016 2:08:37 PM Inj : 1  
Inj Volume : 3.000 µl  
Acq. Method : D:\AGLIENT 1260\DATA\20160506\20160506 2016-05-06 08-43-06\100-1000MS+3MIN-  
1.5\_(0.02%FA).M  
Last changed : 5/6/2016 8:43:06 AM by Su Xiao Ying(LCMS-02)  
Analysis Method : D:\AGLIENT 1260\DATA\20160506\20160506 2016-05-06 08-43-06\100-1000MS+3MIN-  
1.5\_(0.02%FA).M (Sequence Method)  
Last changed : 5/6/2016 2:12:50 PM by Su Xiao Ying(LCMS-02)  
(modified after loading)  
Method Info : HY-365\_5H01RS,M,A-RP-108, 210nm,23min  
Catalog No : HY-10943 Batch#20311  
A-RP-134

Additional Info : Peak(s) manually integrated

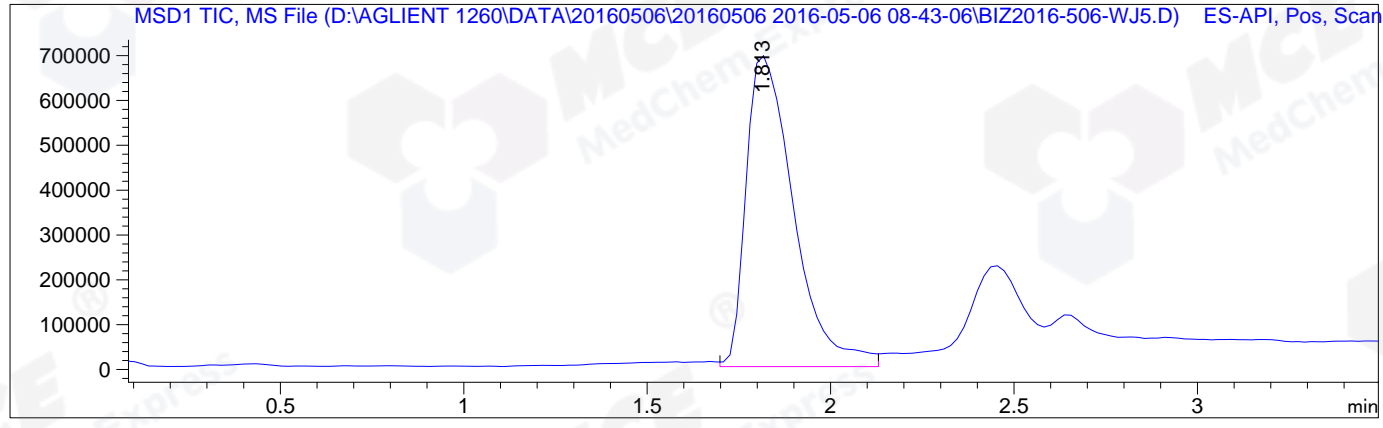

MS Signal: MSD1 TIC, MS File, ES-API, Pos, Scan, Frag: 50  
Spectra averaged over upper half of peaks.  
Noise Cutoff: 1000 counts.  
Reportable Ion Abundance: > 10%.

Retention Time (MS)	MS Area	Mol. Weight or Ion
1.813	6255870	549.30 I
		548.25 I
		274.65 I

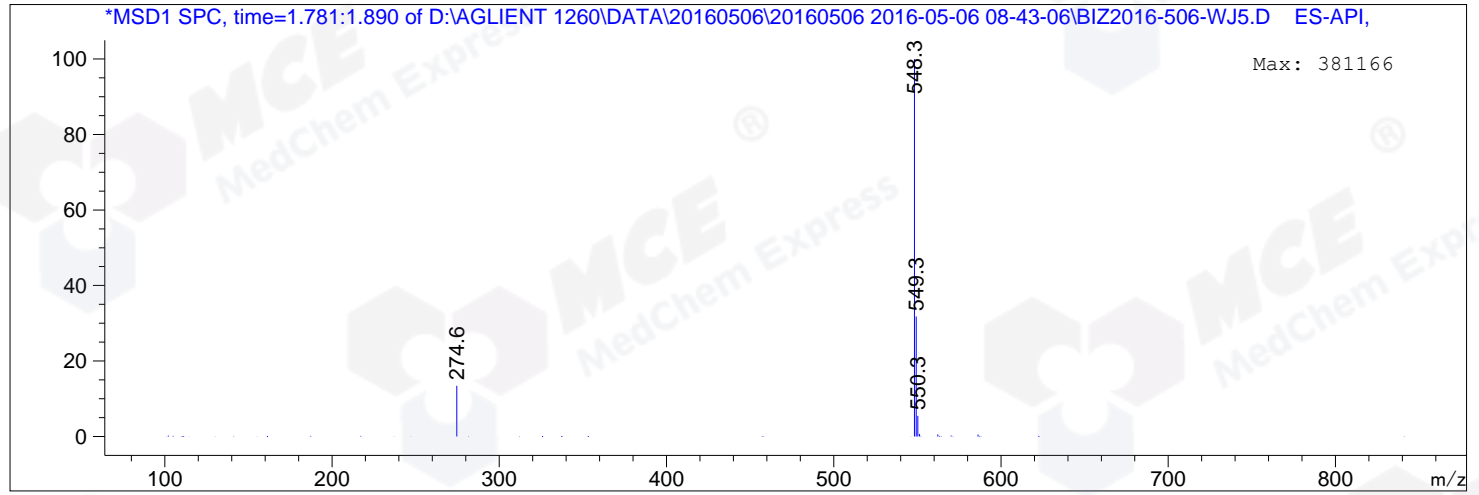

\*\*\* End of Report \*\*\*