



File ..\DATA\2020\20200518\963\CPK2020-515-30187.D Tgt Mass (CHM):  
Injection Date : 18 May 20 3:42 pm +0800 Seq. Line : 50  
Sample Name : CPK2020-515-30187 Location : P1-D-01  
Acq. Operator : ZJ\_1432 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20200518\963\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200518\963\1-POS-3MIN.M  
Catalog No : HY-109565  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

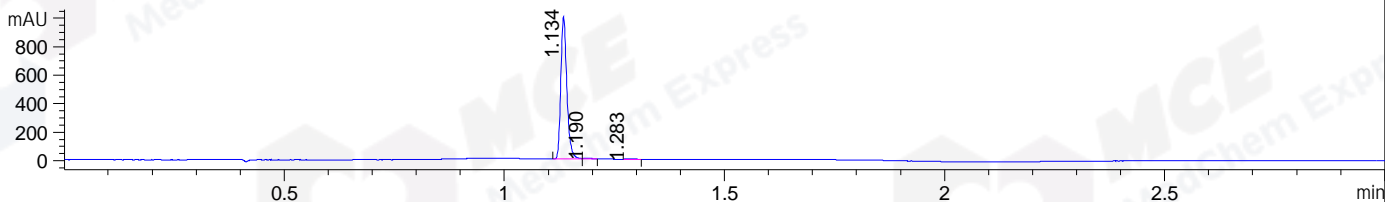


DAD1 C, Sig=254,4 Ref=off

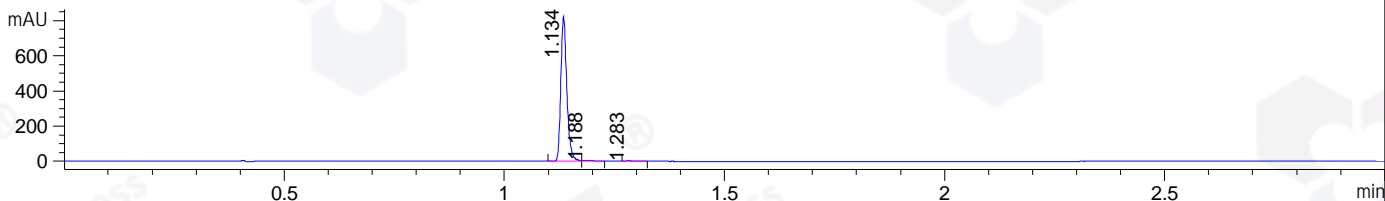

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

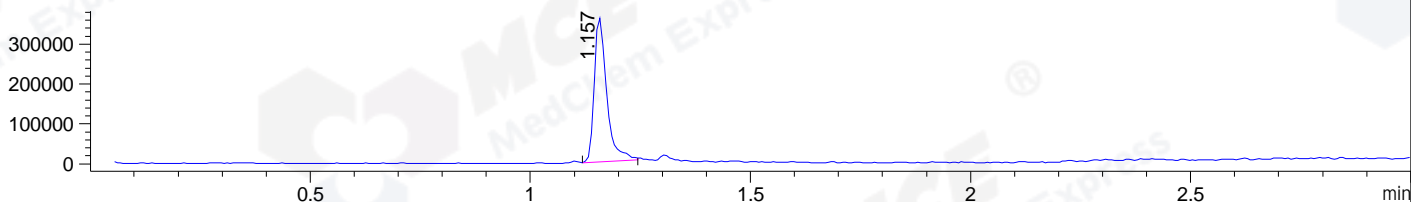

Ion 540, MSD1 540, Target Mass 539 +H Positive, EIC=539.7:540.7

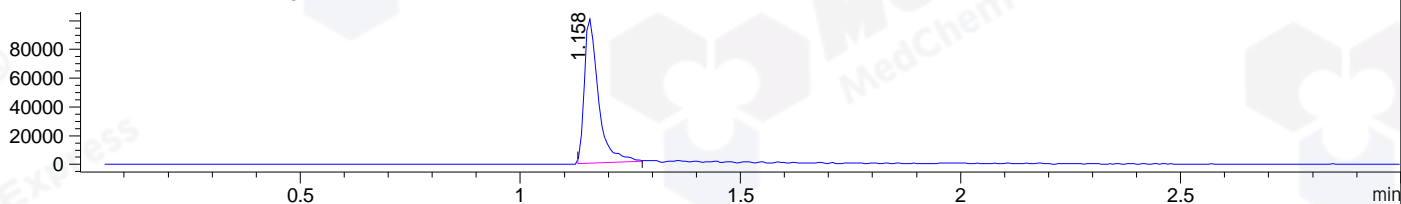

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.02	950.89	1000.22	99.01	271
1.19	0.02	6.88	5.72	0.72	540
1.28	0.02	2.65	2.60	0.28	540

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.02	778.73	824.74	98.64	271
1.19	0.02	7.06	5.27	0.89	540
1.28	0.02	3.66	2.85	0.46	596

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.16	0.03	712490.75	362178.06	100.00	271

Ret. Time: 1.16

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

