



File ..\DATA\2020\20201023\1135\BIZ2020-O22-SCH7.D Tgt Mass (CHM):
Injection Date : 23 Oct 20 4:14 pm +0800 Seq. Line : 47
Sample Name : BIZ2020-O22-SCH7 Location : P1-B-02
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201023\1135\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201023\1135\1-POS-3MIN.M
Catalog No : HY-10957
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

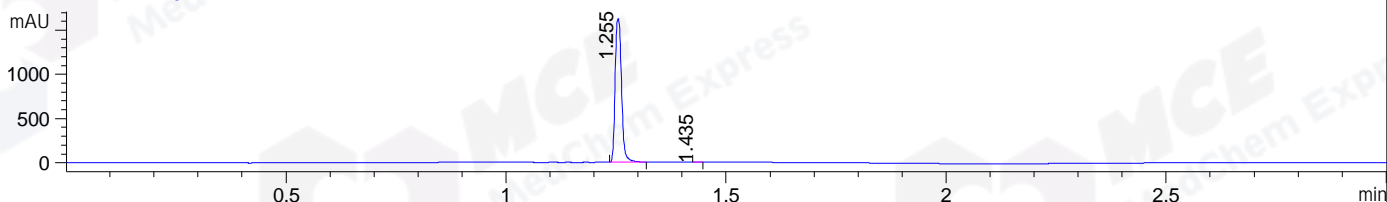


DAD1 C, Sig=254,4 Ref=off

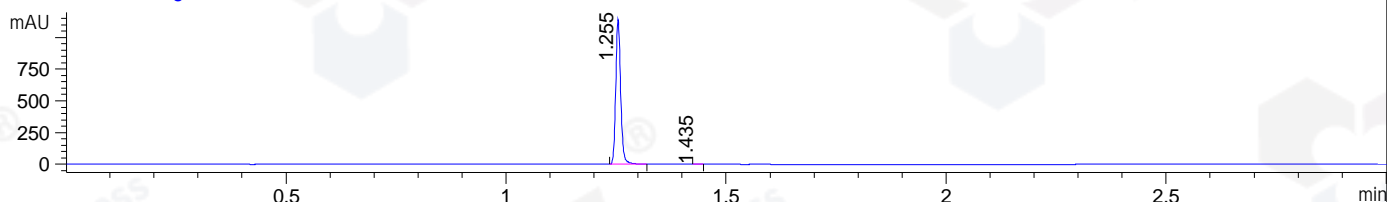

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

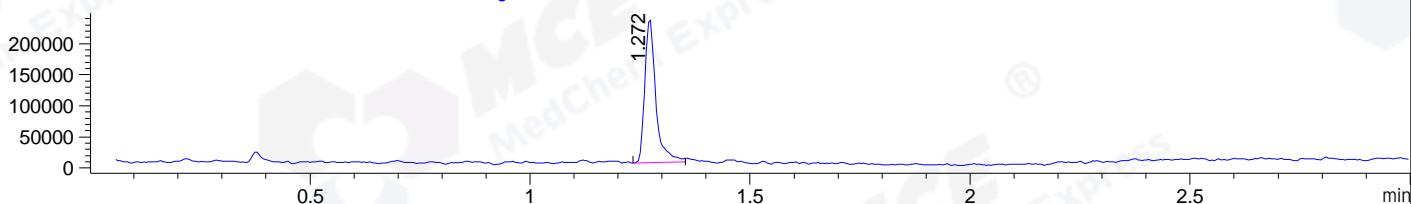

Ion 510, MSD1 510, Target Mass 509 +H Positive, EIC=509.7:510.7

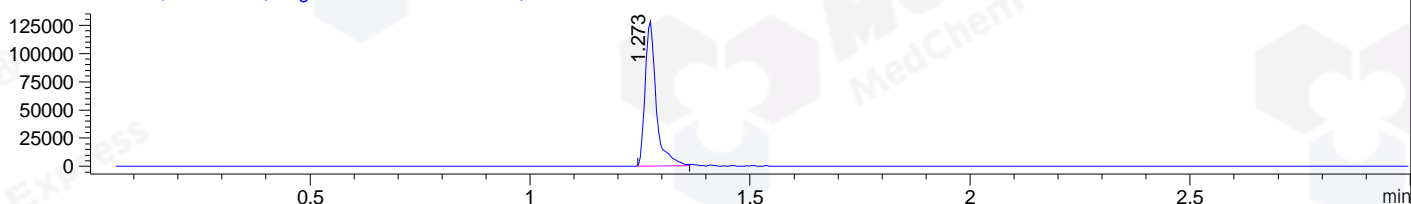

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.25	0.02	1637.51	1626.19	99.88	510
1.44	0.01	2.03	2.80	0.12	157

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.25	0.01	894.86	1143.74	99.92	510
1.44	0.01	0.71	1.03	0.08	157

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.27	0.03	404440.97	232651.06	100.00	510

Ret. Time: 1.27

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

