



File ..DATA\2021\20210207\1274\CPK2021-207-03615.D Tgt Mass (CHM):
Injection Date : 7 Feb 21 2:43 pm +0800 Seq. Line : 66
Sample Name : CPK2021-207-03615 Location : P1-E-06
Acq. Operator : yrz_1364 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2021\20210207\1274\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2021\20210207\1274\1-POS-3MIN.M
CAS NO. : 405554-55-4
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

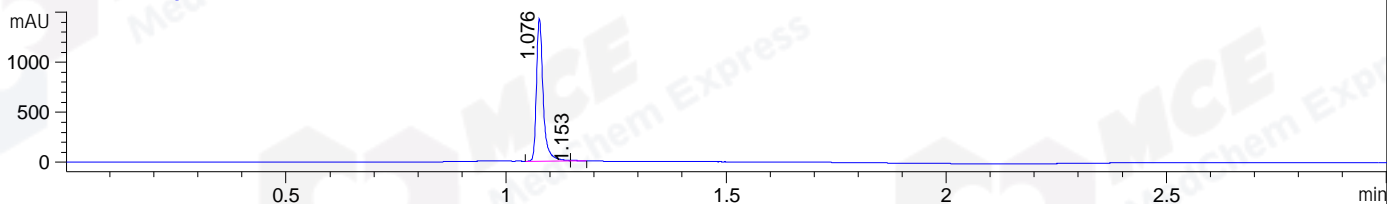


DAD1 C, Sig=254,4 Ref=off

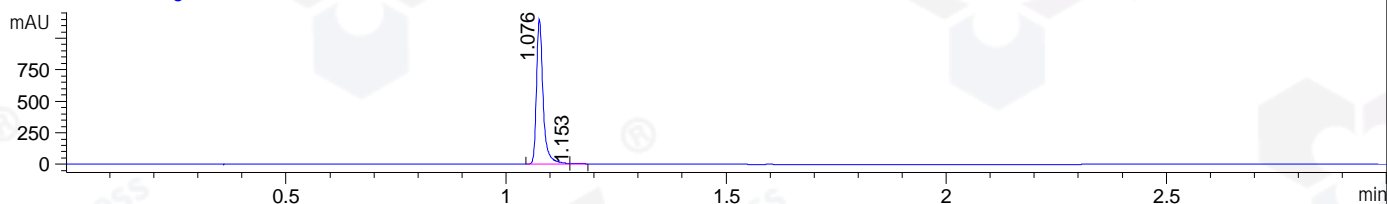

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

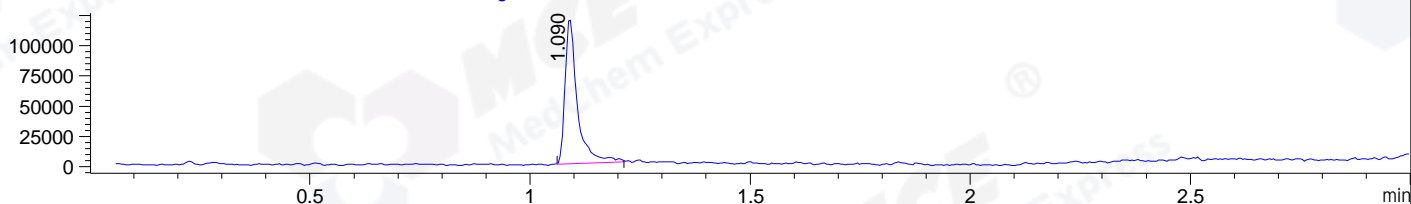

Ion 454, MSD1 454, Target Mass 453 +H Positive, EIC=453.7:454.7

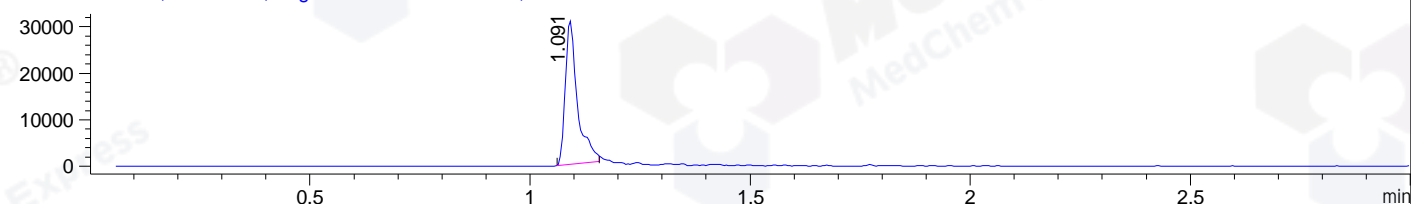

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.02	1509.39	1426.81	99.56	228
1.15	0.02	6.68	5.06	0.44	454

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.02	1201.64	1149.97	99.52	228
1.15	0.02	5.78	4.26	0.48	454

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.03	233155.03	120694.02	100.00	228

Ret. Time: 1.09

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

