



File ..019\20190703\20190703 1\CPK2019-702-30987.D Tgt Mass (CHM):  
 Injection Date : 3 Jul 19 5:55 pm +0800 Seq. Line : 76  
 Sample Name : CPK2019-702-30987 Location : P2-D-03  
 Acq. Operator : SYSTEM Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\LCMS03\Data\20190703\20190703 1\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2019\20190703\20190703 1\1-POS-3MIN.M  
 Catalog No : HY-10999 Batch#30987  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-446  
 Oven Temperature : 45C


DAD1 B, Sig=254,4 Ref=off

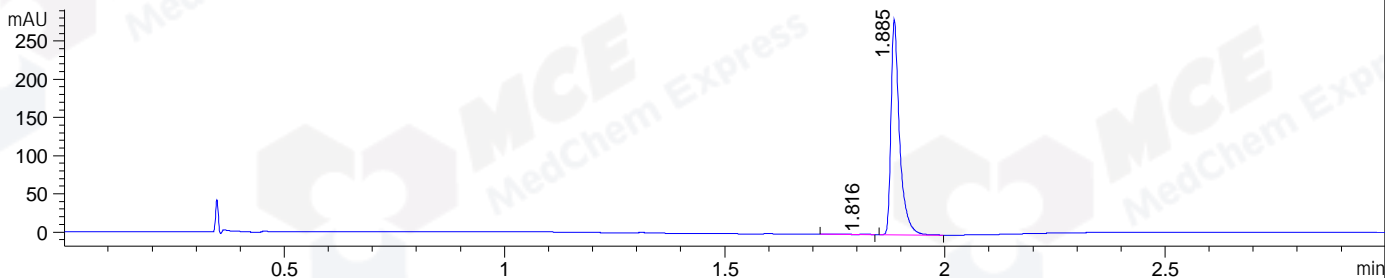

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

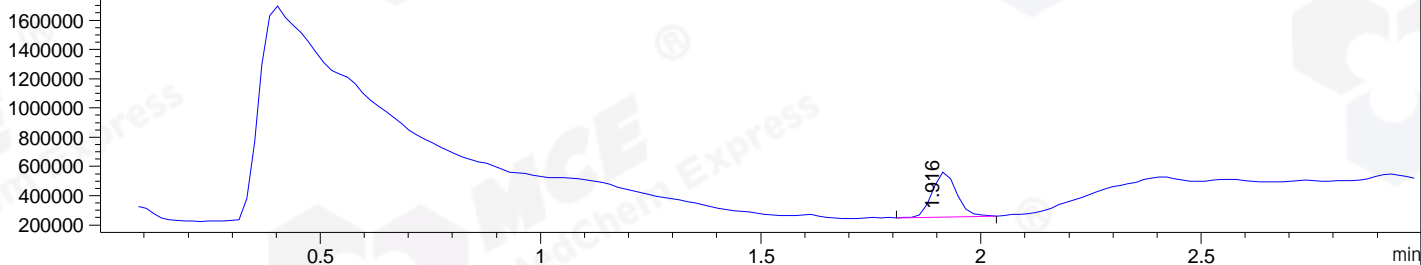

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

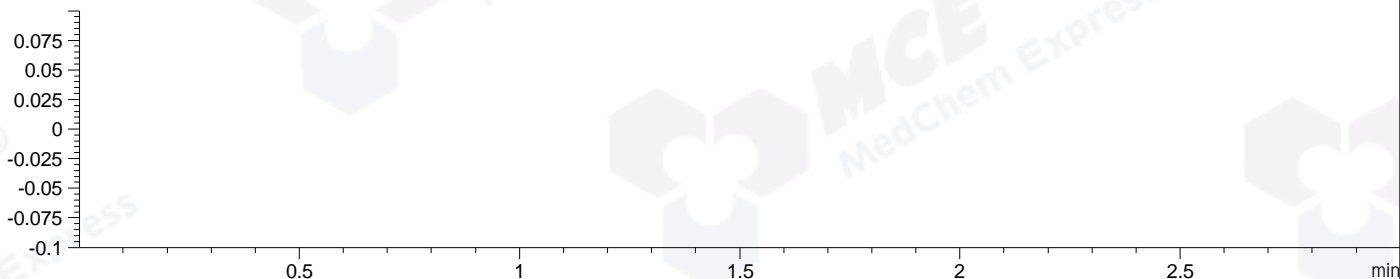

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.82	0.05	2.16	0.72	0.56	145
1.89	0.02	381.21	281.43	99.44	616

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.92	0.06	1183592.50	309646.44	100.00	145

Ret. Time: 1.92

<<<< POSITIVE SPECTRA >>>>

