

File ..\DATA\2020\20200402\910\BIZ2020-331-SCH6-.D Tgt Mass (CHM):

Injection Date : 2 Apr 20 2:55 pm +0800 Seq. Line : 77

Sample Name : BIZ2020-331-SCH6 Location : PL-B-04

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.25 ul

Acq. Method : D:\Chem32\1\data\2020\20200402\910\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200402\910\1-POS-3MIN.M

Catalog No : HY-110084 Batch#62148

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

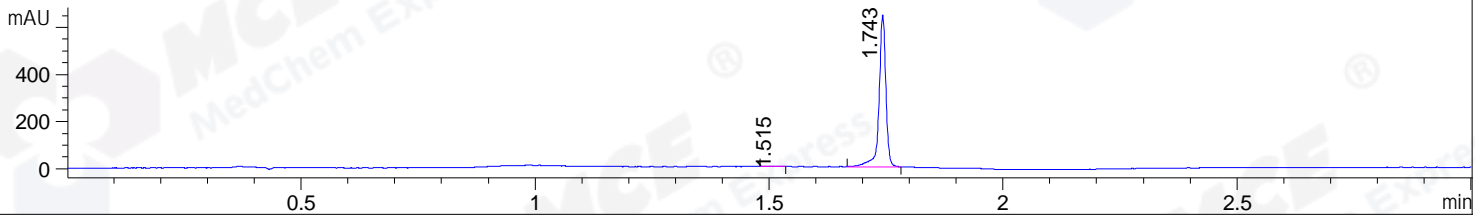


DAD1 C, Sig=254,4 Ref=off

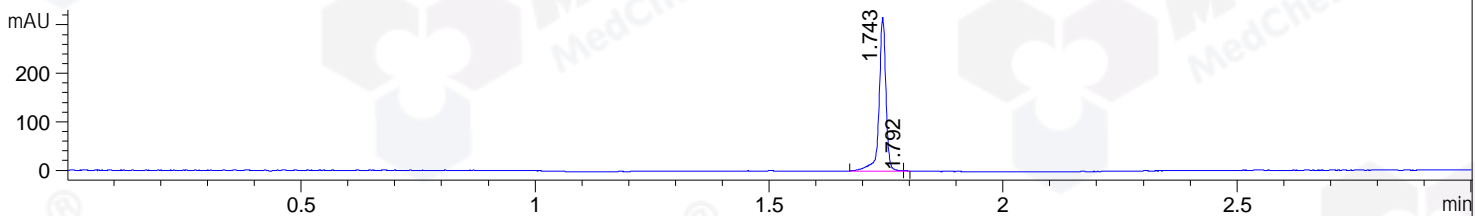

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

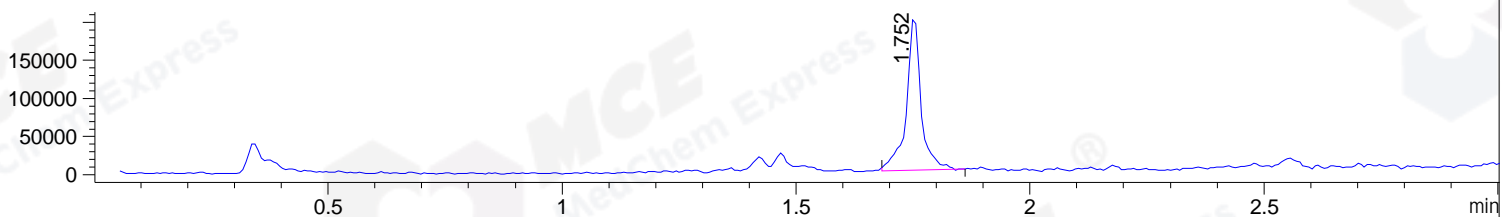

Ion 241, MSD1 241, Target Mass 240 +H Positive, EIC=240.7:241.7

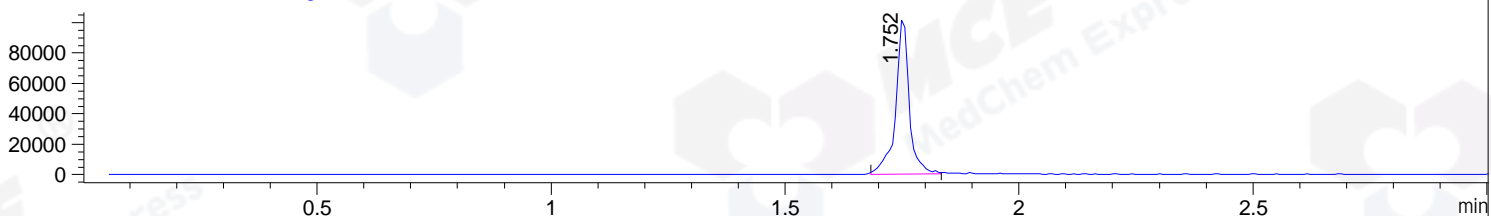

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.03	2.84	1.60	0.43	491
1.74	0.02	654.62	646.18	99.57	241

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.74	0.02	322.09	317.92	99.92	241
1.79	0.01	0.26	0.53	0.08	241

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.75	0.03	433864.78	203031.53	100.00	241

Ret. Time: 1.75

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

