



File ..DATA\2020\20201013\1124\CPK2020-O13-15608.D Tgt Mass (CHM):
Injection Date : 13 Oct 20 5:02 pm +0800 Seq. Line : 71
Sample Name : CPK2020-O13-15608 Location : P1-D-01
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201013\1124\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201013\1124\1-POS-3MIN.M
Catalog No : HY-11068
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

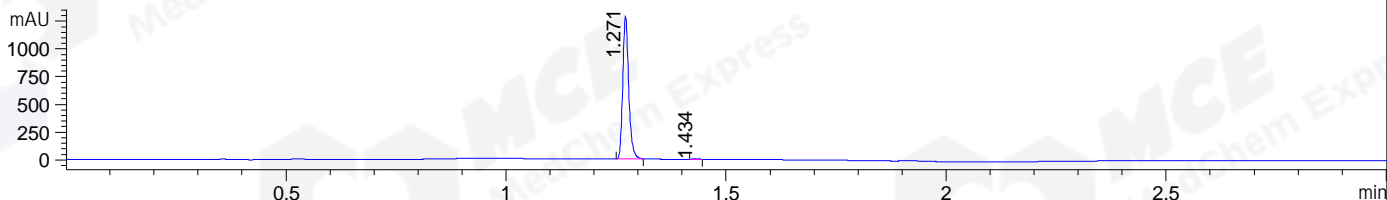


DAD1 C, Sig=254,4 Ref=off

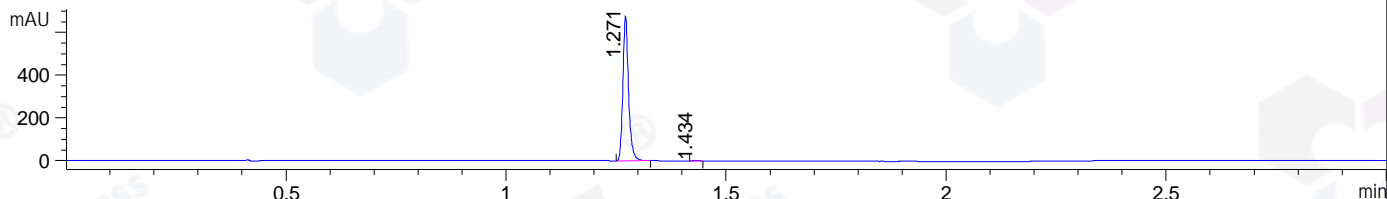

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

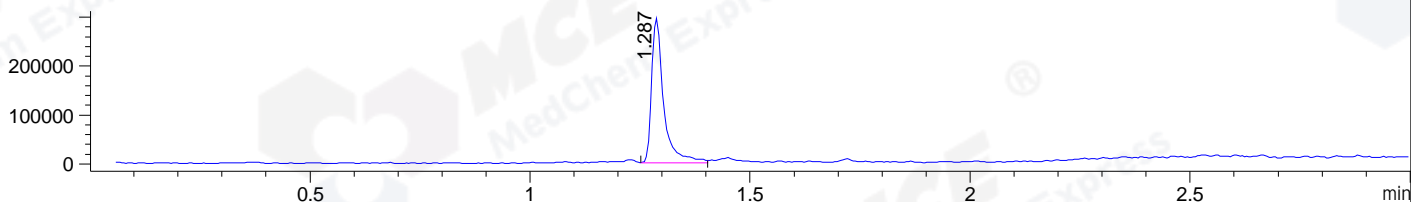

Ion 369, MSD1 369, Target Mass 368 +H Positive, EIC=368.7:369.7

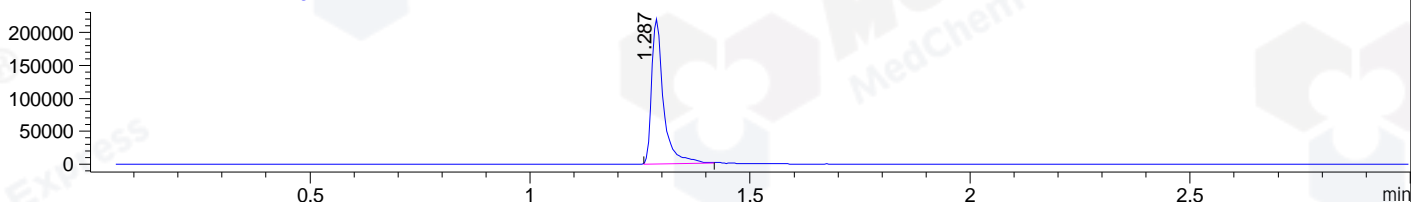

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.27	0.02	1210.16	1284.14	99.80	369
1.43	0.02	2.47	2.51	0.20	369

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.27	0.01	607.64	676.13	99.80	369
1.43	0.02	1.23	1.23	0.20	369

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.29	0.03	566584.94	295999.50	100.00	369

Ret. Time: 1.29

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

