
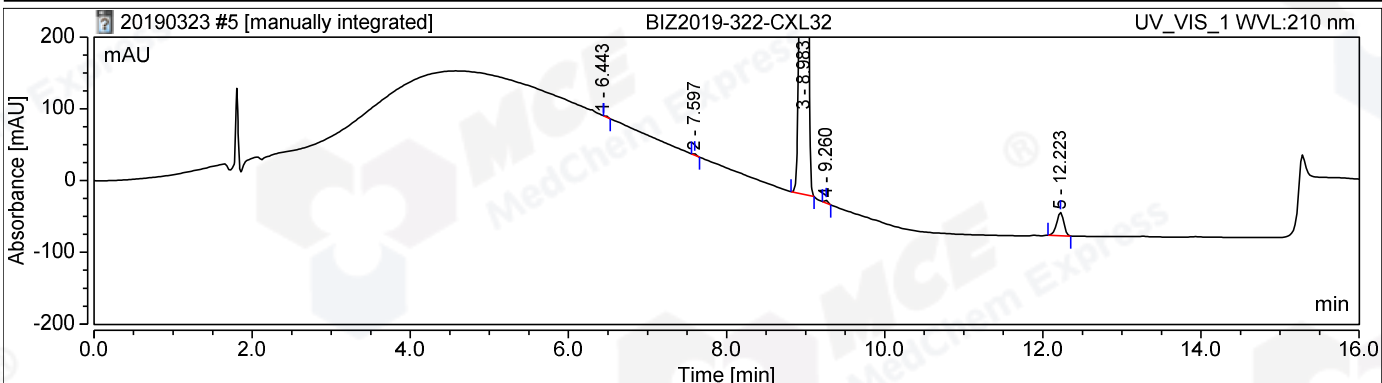


### Chromatogram and Results

#### Injection Details

<b>Injection Name:</b> BIZ2019-322-CXL32	<b>Run Time (min):</b> 16.00
<b>Vial Number:</b> BA7	<b>Users:</b> zqq
<b>Injection Type:</b> Unknown	<b>Injection Volume:</b> 2.00
<b>Calibration Level:</b>	<b>Channel:</b> UV_VIS_1
<b>Instrument Method:</b> 10-90A 214NM	<b>Wavelength:</b> 210
<b>Processing Method:</b> New processing	<b>Bandwidth:</b> 4
<b>Comment:</b> HY-111363-20190322 A-RP-328	<b>Dilution Factor:</b> 1.0000
<b>Injection Date/Time:</b> 23/Mar/19 17:48	<b>Sample Weight:</b> 1.0000

#### Chromatogram

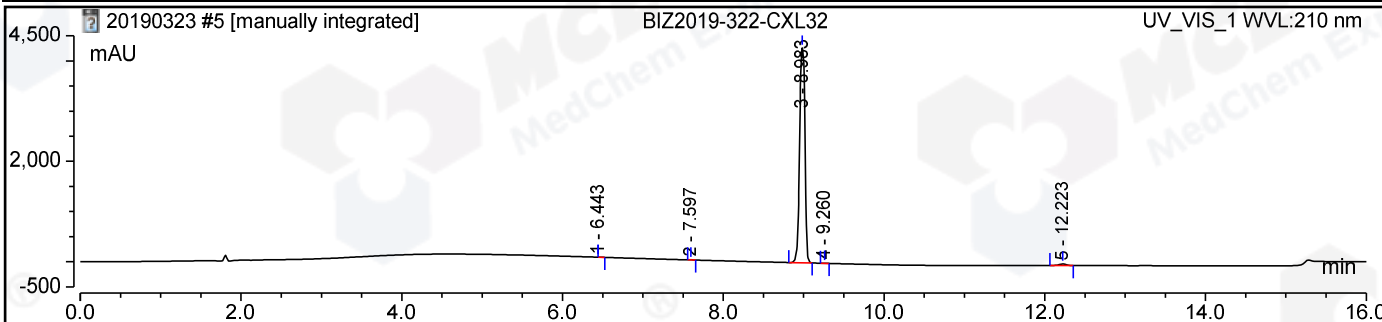

#### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
1		6.443	0.052	0.000	n.a.	1000	n.a.	0.02
2		7.597	0.092	2.080	14.34	999	1.23	0.03
3		8.983	328.223	4277.236	2.68	977	0.93	98.87
4		9.260	0.195	3.847	23.81	999	1.09	0.06
5		12.223	3.421	32.433	n.a.	1000	0.91	1.03
Total:			331.983	4315.596	40.83			4.15