

File ..1\DATA\2019\20190315\557\BIZ2019-314-WYQ6.D Tgt Mass (CHM):

Injection Date : 15 Mar 19 12:00 pm +0800 Seq. Line : 33

Sample Name : BIZ2019-314-WYQ6 Location : P1-D-07

Acq. Operator : LQ\_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190315\557\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190315\557\1-POS-3MIN-1.M

Catalog No : HY-111617 Batch#39161

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

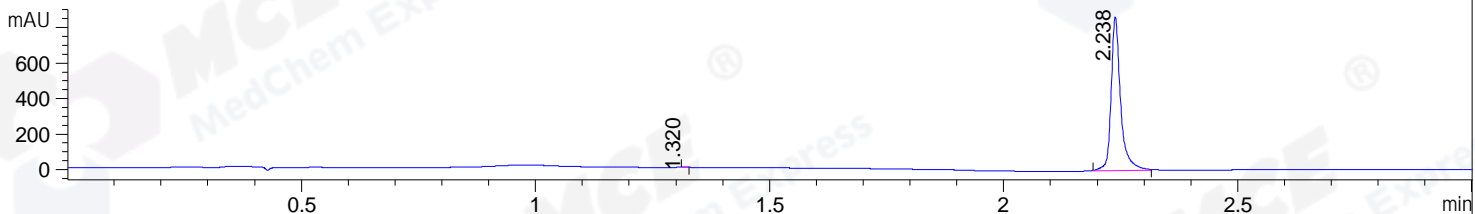


DAD1 C, Sig=254,4 Ref=off

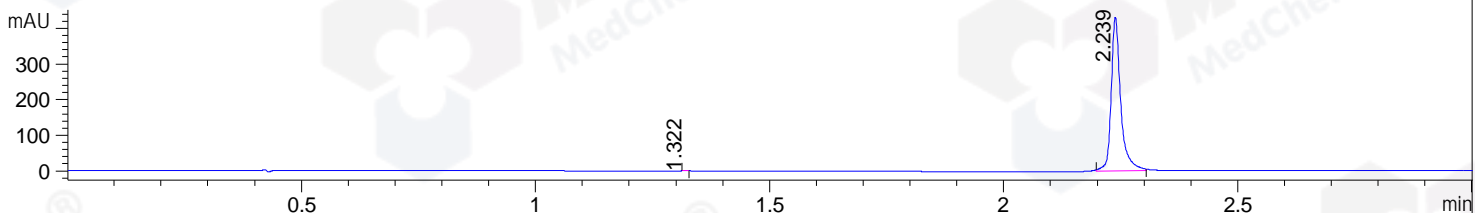

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

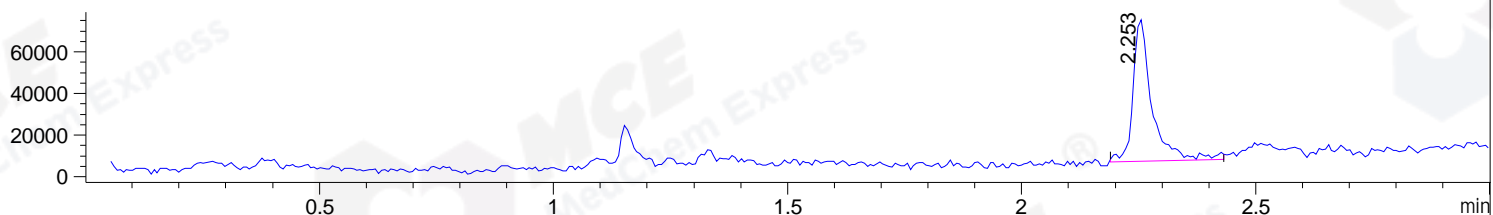

Ion 250, MSD1 250, Target Mass 249 +H Positive, EIC=249.7:250.7

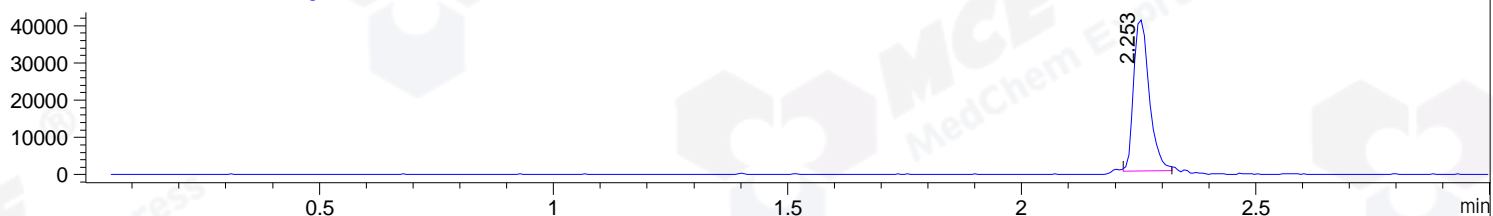

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.32	0.01	0.50	0.91	0.04	ND
2.24	0.02	1234.34	867.36	99.96	250

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.32	0.01	0.26	0.42	0.04	ND
2.24	0.02	610.68	431.22	99.96	250

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.25	0.04	193393.50	68495.28	100.00	250

Ret. Time: 2.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

