

File ..1\DATA\2019\20190507\570\BIZ2019-506-WYQ2.D Tgt Mass (CHM):

Injection Date : 7 May 19 5:30 pm +0800 Seq. Line : 18

Sample Name : BIZ2019-506-WYQ2 Location : PL-F-01

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190507\570\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190507\570\1-POS-3MIN-1.M

Catalog No : HY-111802 Batch#40783 BY DMSO

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-322

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

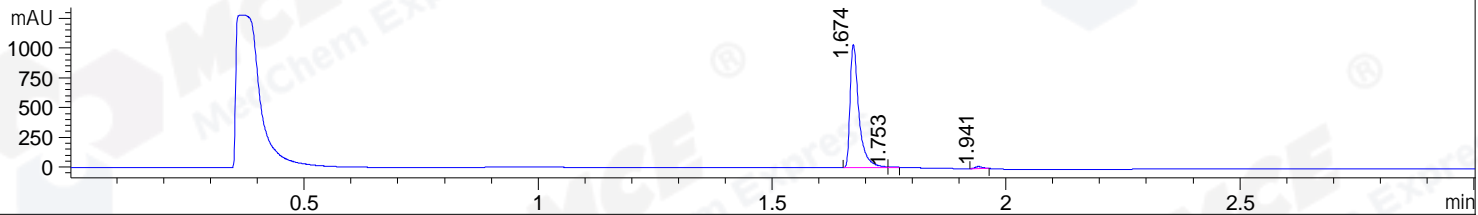


DAD1 C, Sig=254,4 Ref=off

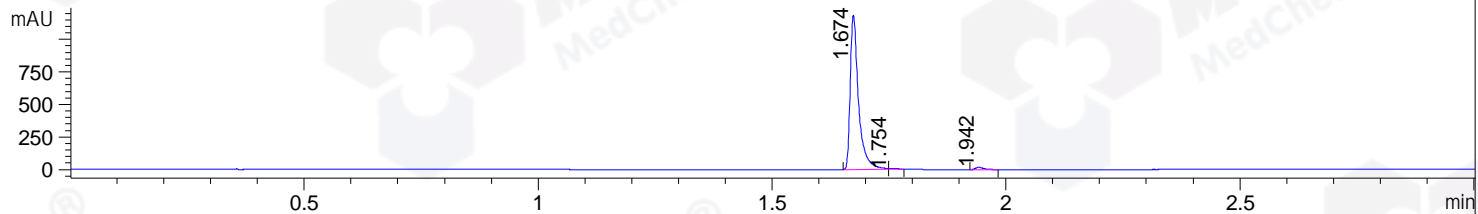

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

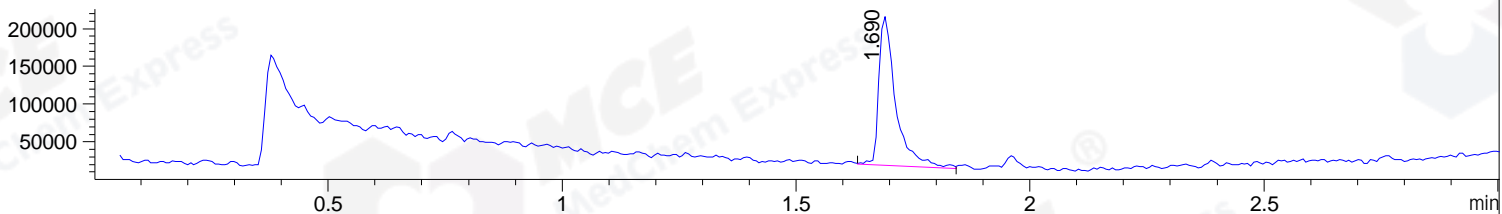

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

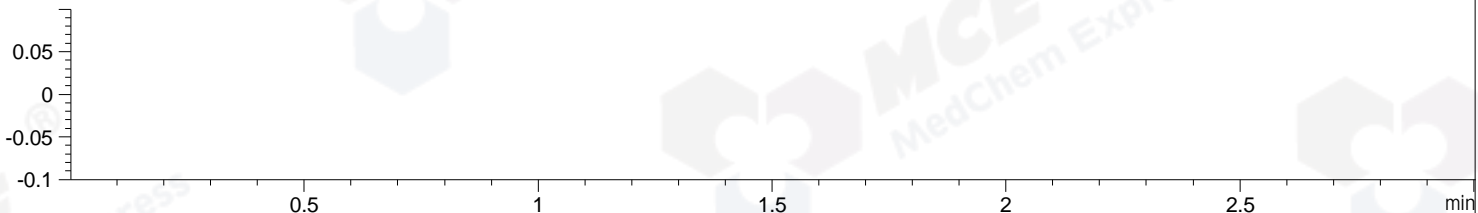

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.67	0.02	1353.88	1034.05	98.20	255
1.75	0.02	5.54	5.86	0.40	157
1.94	0.02	19.30	17.50	1.40	157

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.67	0.02	1460.38	1186.04	97.87	255
1.75	0.02	7.56	6.97	0.51	157
1.94	0.02	24.28	18.48	1.63	157

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.69	0.04	495923.97	197608.69	100.00	255

Ret. Time: 1.69

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

