


Chromatogram and Results

Injection Details

Injection Name: FSD6718-040-2A	Injection Volume: 5.00
Vial Number: RA2	Channel: UV_VIS_1
Injection Type: Unknown	Wavelength: 230
Calibration Level:	Users: zqq
Instrument Method: HM-646_16-H01P01(RP-HPLC)	Dilution Factor: 1.0000
Processing Method: New Processing Method	Sample Weight: 1.0000
Injection Date/Time: 29/Jul/19 15:05	Run Time (min): 30.00
Comment: HM-646_16-20190711 A-RP-333	

chrom://hy261/ChromeleonLocal/Chemistry Analy/201907/20190729.seq/481.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

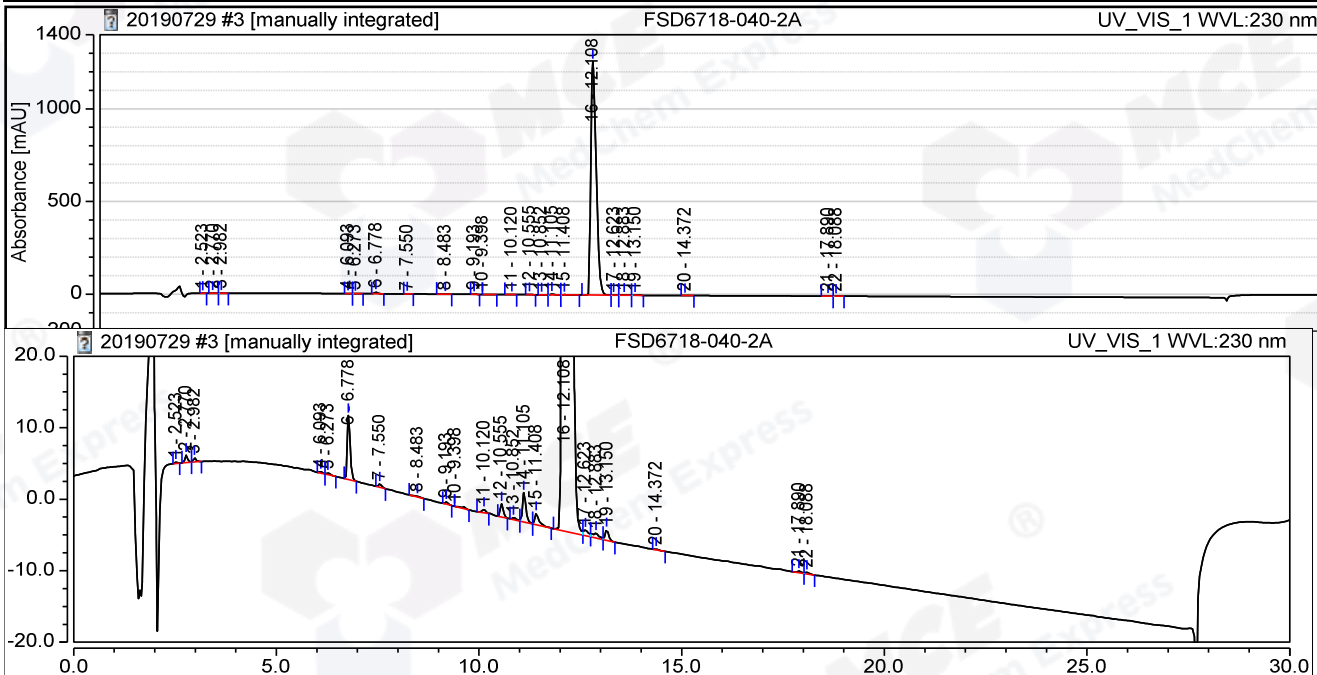

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		2.523	0.012	0.181	1.24	2.34	0.01
2		2.770	0.079	1.048	1.38	1.80	0.04
3		2.982	0.045	0.554	1.26	24.45	0.02
4		6.093	0.019	0.218	n.a.	1.22	0.01
5		6.273	0.027	0.250	n.a.	3.53	0.01
6		6.778	0.723	8.948	1.41	5.88	0.37
7		7.550	0.042	0.464	1.38	4.69	0.02
8		8.483	0.019	0.107	0.87	3.64	0.01
9		9.193	0.025	0.301	1.34	2.87	0.01
10		9.398	0.035	0.010	1.36	8.87	0.02
11		10.120	0.050	0.493	0.89	3.06	0.03
12		10.555	0.158	1.842	1.31	1.73	0.08
13		10.852	0.036	0.290	n.a.	1.43	0.02
14		11.105	0.394	4.094	1.38	2.00	0.20
15		11.408	0.188	1.605	1.86	3.42	0.10
16		12.108	193.554	1258.410	1.69	n.a.	98.81
17		12.623	0.112	0.813	n.a.	n.a.	0.06
18		12.883	0.133	0.708	n.a.	n.a.	0.07
19		13.150	0.157	1.512	n.a.	7.80	0.08
20		14.372	0.010	0.101	1.51	18.85	0.01
21		17.890	0.030	0.223	n.a.	0.94	0.02
22		18.088	0.028	0.228	n.a.	n.a.	0.01
Total:			195.876	1282.400	18.88	98.53	