



File ..\DATA\2019\20190618\594\BIZ2019-617-WYQ21.D Tgt Mass (CHM):
 Injection Date : 18 Jun 19 11:21 am +0800 Seq. Line : 28
 Sample Name : BIZ2019-617-WYQ21 Location : P1-A-08
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190618\594\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190618\594\1-POS-3MIN.M
 Catalog No : HY-112233 Batch#42421
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

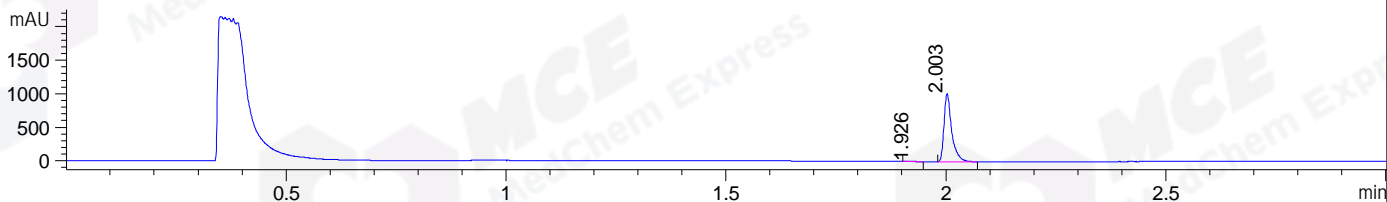


DAD1 C, Sig=254,4 Ref=off

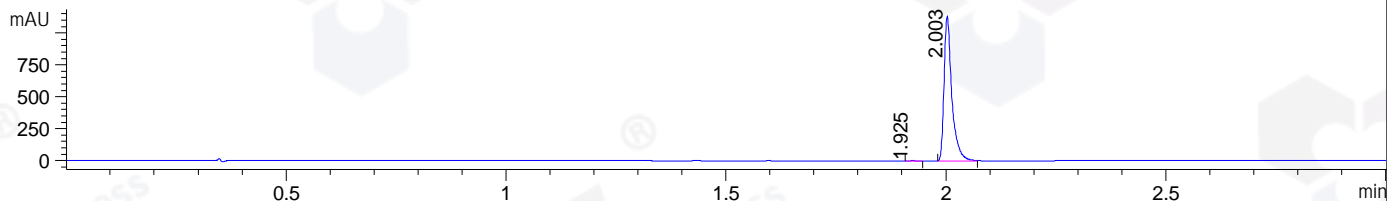

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

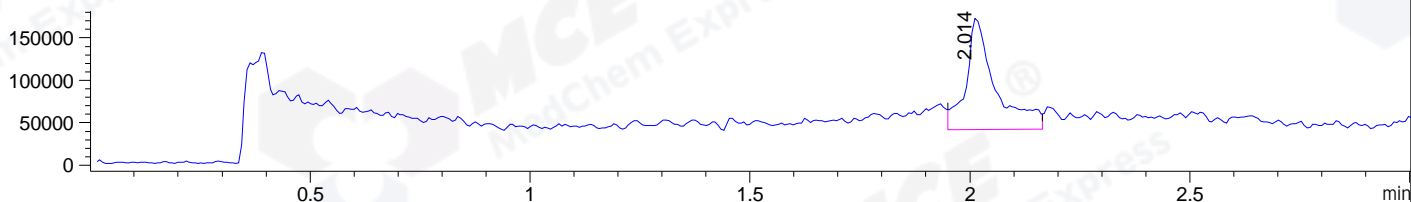

Ion 379.9, MSD1 379.9, Target Mass 378.9 +H Positive, EIC=379.6:380.6

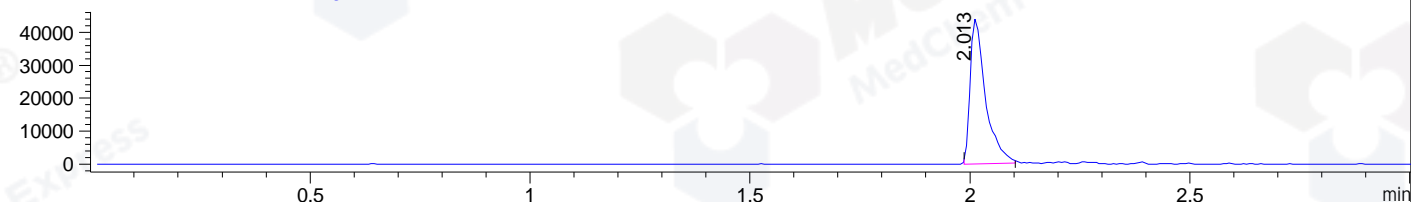

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.93	0.02	3.52	3.60	0.28	157
2.00	0.02	1242.91	1013.55	99.72	157

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.92	0.02	2.62	2.84	0.19	157
2.00	0.02	1398.07	1134.97	99.81	157

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.01	0.06	609993.06	132131.03	100.00	157

Ret. Time: 2.01

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

