



File ..DATA\2021\20210330\1319\CPK2021-329-32610.D Tgt Mass (CHM):  
Injection Date : 30 Mar 21 4:19 pm +0800 Seq. Line : 92  
Sample Name : CPK2021-329-32610 Location : P1-B-06  
Acq. Operator : yrz\_1364 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2021\20210330\1319\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2021\20210330\1319\1-POS-3MIN.M  
CAS NO. : 1442472-39-0  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

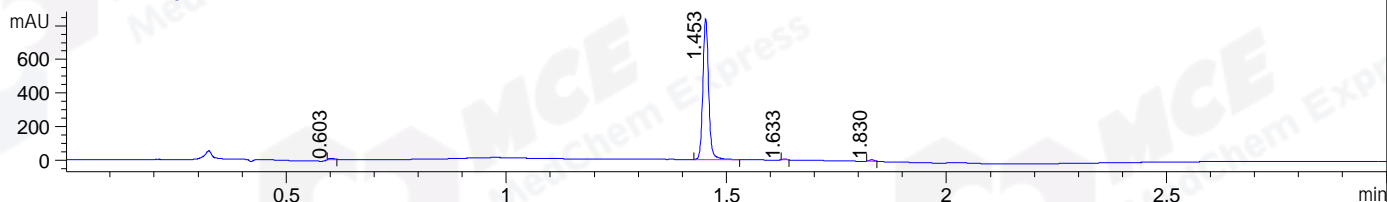


DAD1 C, Sig=254,4 Ref=off

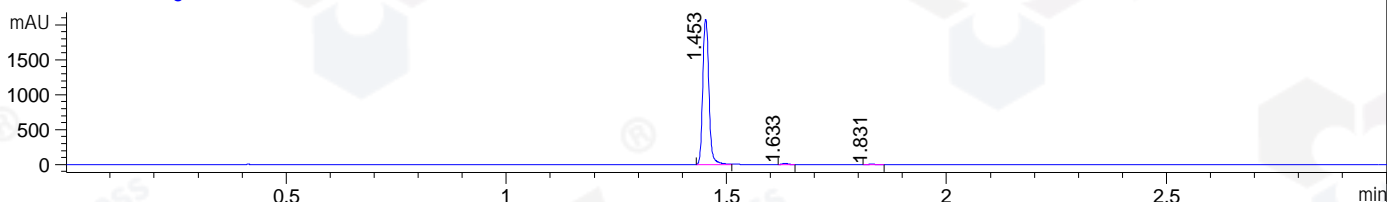

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

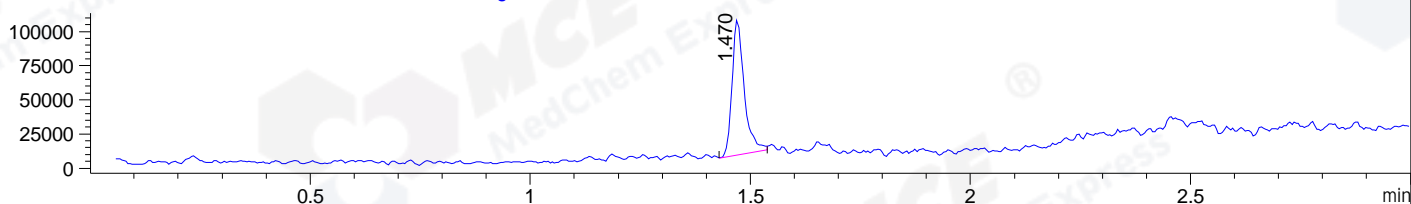

Ion 510, MSD1 510, Target Mass 509 +H Positive, EIC=509.7:510.7

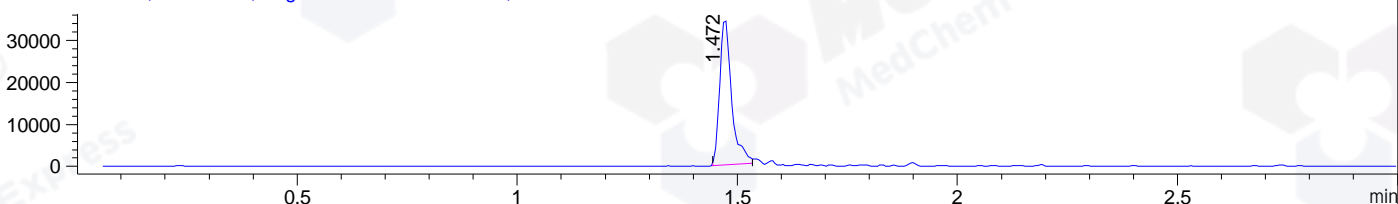

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.60	0.01	5.30	7.18	0.68	ND
1.45	0.02	761.45	840.26	98.05	510
1.63	0.01	3.59	5.14	0.46	ND
1.83	0.01	6.23	7.91	0.80	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.45	0.02	2019.47	2079.72	98.86	510
1.63	0.01	14.66	16.90	0.72	ND
1.83	0.02	8.68	7.88	0.42	ND


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.47	0.03	190835.89	98902.87	100.00	510

Ret. Time: 1.47

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

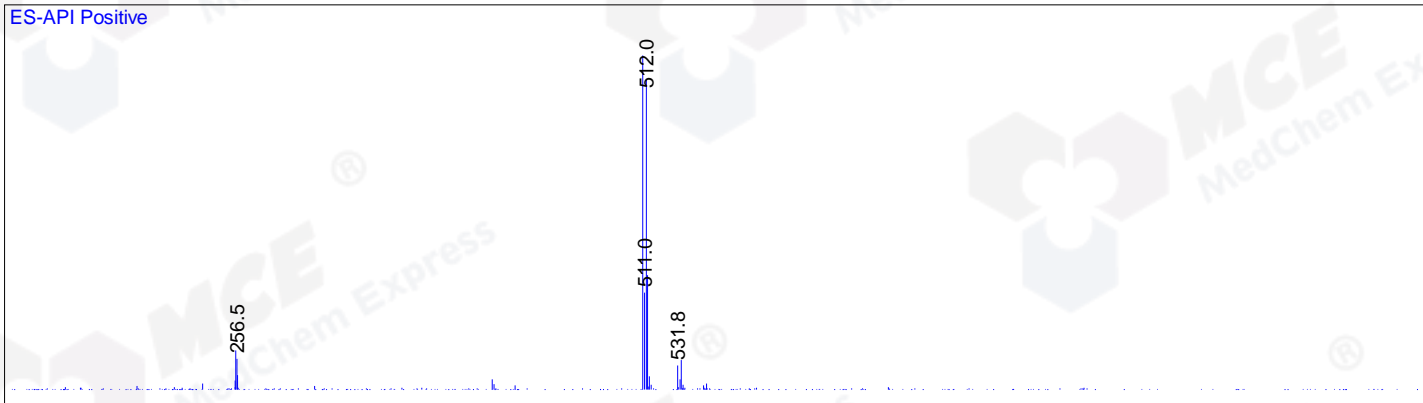

MS Spectrum

MSD1 SPC, time=1.479 of D:\CHEM32\1\DATA\2021\20210330\1319\CPK2021-329-32610.D ES-API, Pos, Scan, Frag: 70

